



Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001016.D
Acq On : 18 Jul 2012 14:36
Operator : HLM
Sample : PB64274BS
Misc : WATER BNA_J HLM
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB64274BS

Quant Time: Jul 23 01:40:54 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:03:32 2012
Response via : Initial Calibration

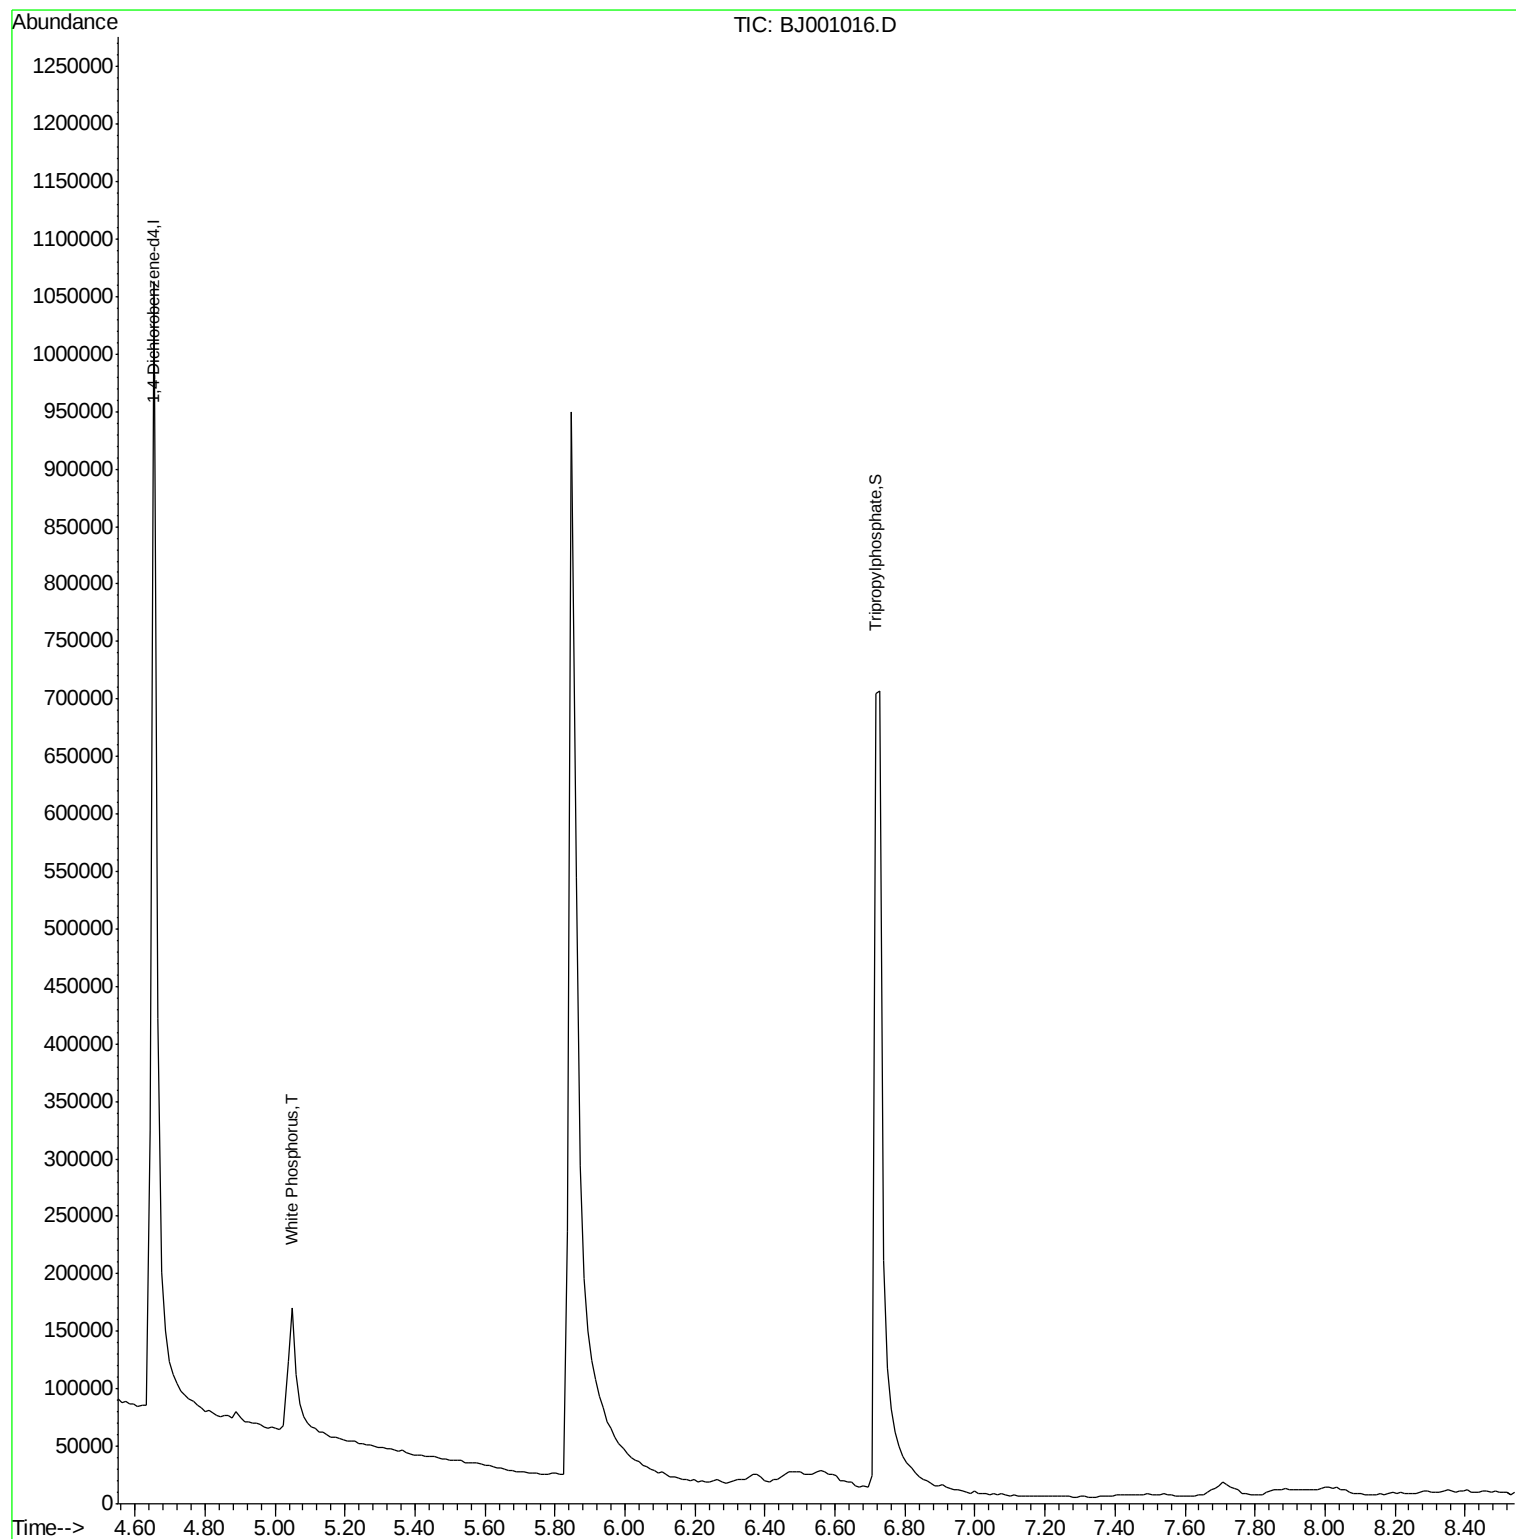

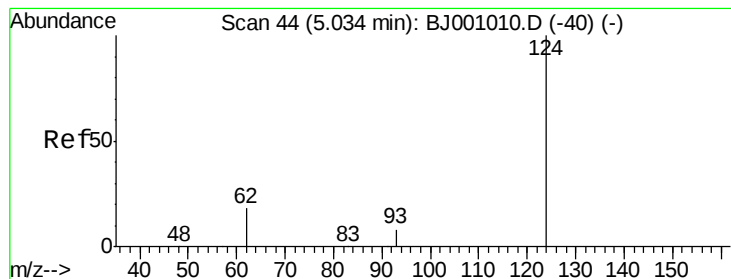

#3

White Phosphorus

Concen: 0.53 ug/ml

RT: 5.05 min Scan# 45

Delta R.T. 0.01 min

Lab File: BJ001016.D

Acq: 18 Jul 2012 14:36

Instrument :

BNA_J

ClientSampleId :

PB64274BS



Tgt Ion:124 Resp: 168900

Ion Ratio Lower Upper

124 100

93 7.6 0.0 27.8


62 20.0 0.0 39.0

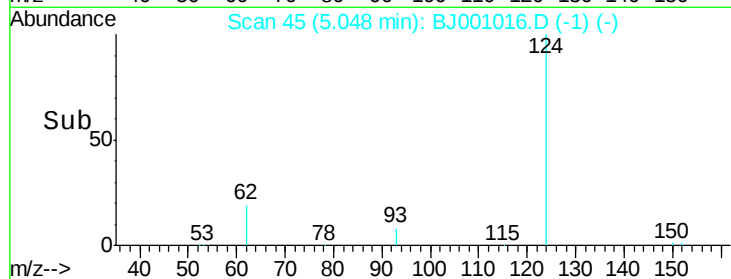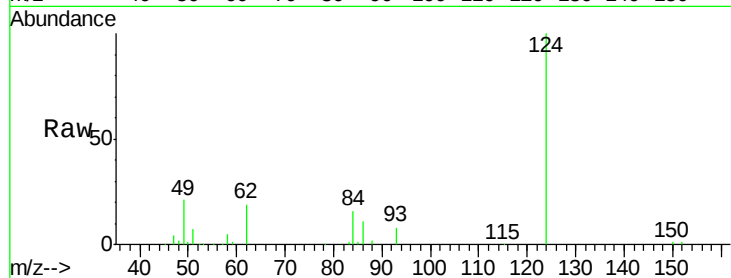

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

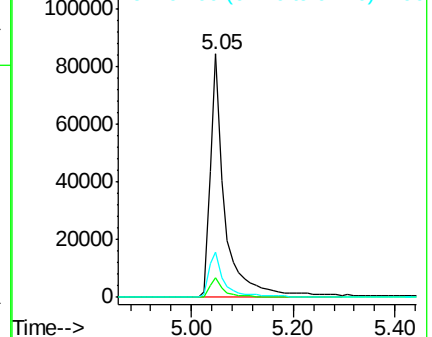

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001016.D
Acq On : 18 Jul 2012 14:36
Operator : HLM
Sample : PB64274BS
Misc : WATER BNA_J HLM
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB64274BS

Quant Time: Jul 23 01:40:54 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:03:32 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.65	150	386175	2.50	ug/ml	0.01

System Monitoring Compounds

2) Tripropylphosphate	6.72	99	757595	2.45	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	98.00%

Target Compounds					Qvalue
3) White Phosphorus	5.05	124	168900	0.53	ug/ml 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed