

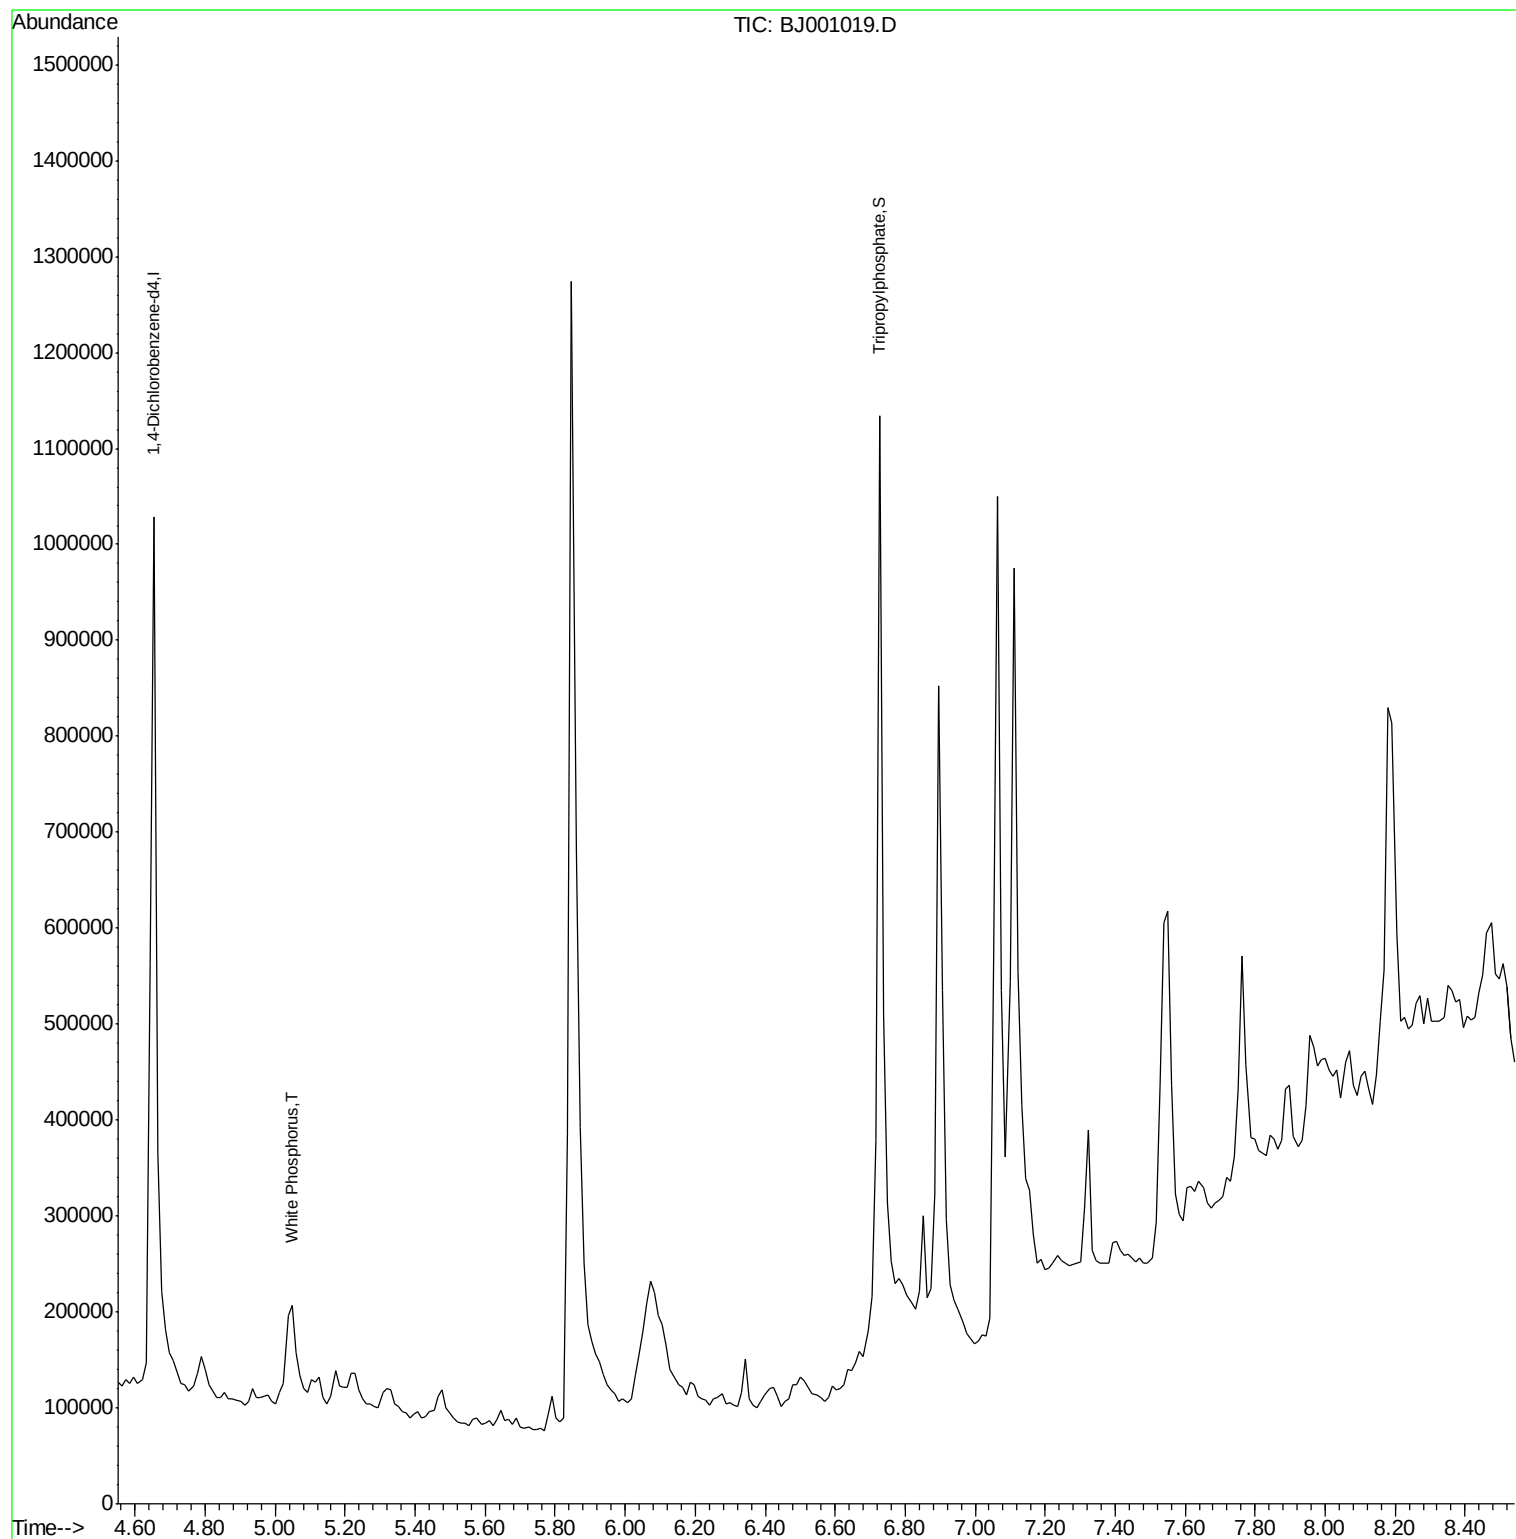
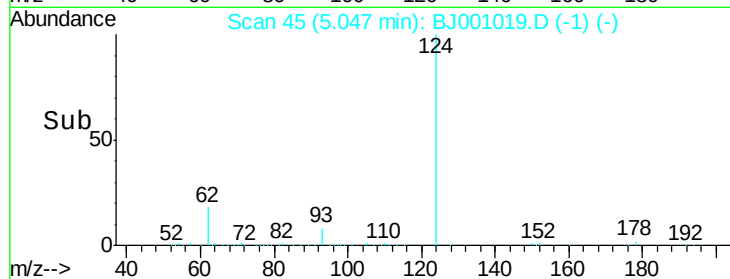


Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001019.D
Acq On : 18 Jul 2012 15:16
Operator : HLM
Sample : D3369-01MSD
Misc : WATER BNA_J HLM
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
RUN 1MSD

Quant Time: Jul 23 01:41:04 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:03:32 2012
Response via : Initial Calibration

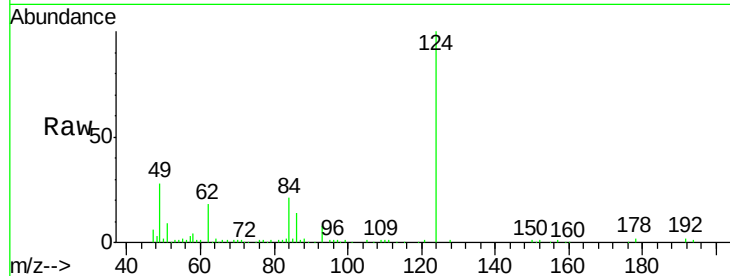

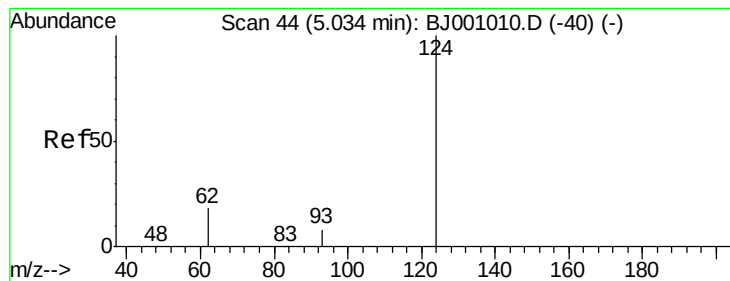

#3

White Phosphorus

Concen: 0.53 ug/ml

RT: 5.05 min Scan# 45

Delta R.T. 0.01 min

Lab File: BJ001019.D

Acq: 18 Jul 2012 15:16

Instrument :

BNA_J

ClientSampleId :

RUN 1MSD

Tgt Ion:124 Resp: 166784

Ion Ratio Lower Upper

124 100


93 9.0 0.0 27.8

62 21.9 0.0 39.0

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

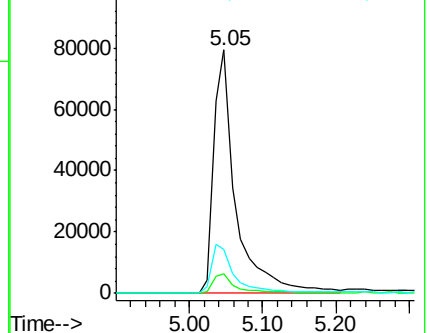

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ071812\
Data File : BJ001019.D
Acq On : 18 Jul 2012 15:16
Operator : HLM
Sample : D3369-01MSD
Misc : WATER BNA_J HLM
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
RUN 1MSD

Quant Time: Jul 23 01:41:04 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Jul 18 14:03:32 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.65	150	381769	2.50	ug/ml	0.01

System Monitoring Compounds

2) Tripropylphosphate	6.73	99	704510	2.30	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	92.00%

Target Compounds					Qvalue
3) White Phosphorus	5.05	124	166784	0.53	ug/ml 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed