



Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ072012\
Data File : BJ001045.D
Acq On : 20 Jul 2012 15:44
Operator : HLM
Sample : D3359-01
Misc : WATER BNA_J HLM
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Jul 21 05:01:09 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ072012.M
Quant Title : CWA degradation products by GCMS
QLast Update : Fri Jul 20 14:08:00 2012
Response via : Initial Calibration

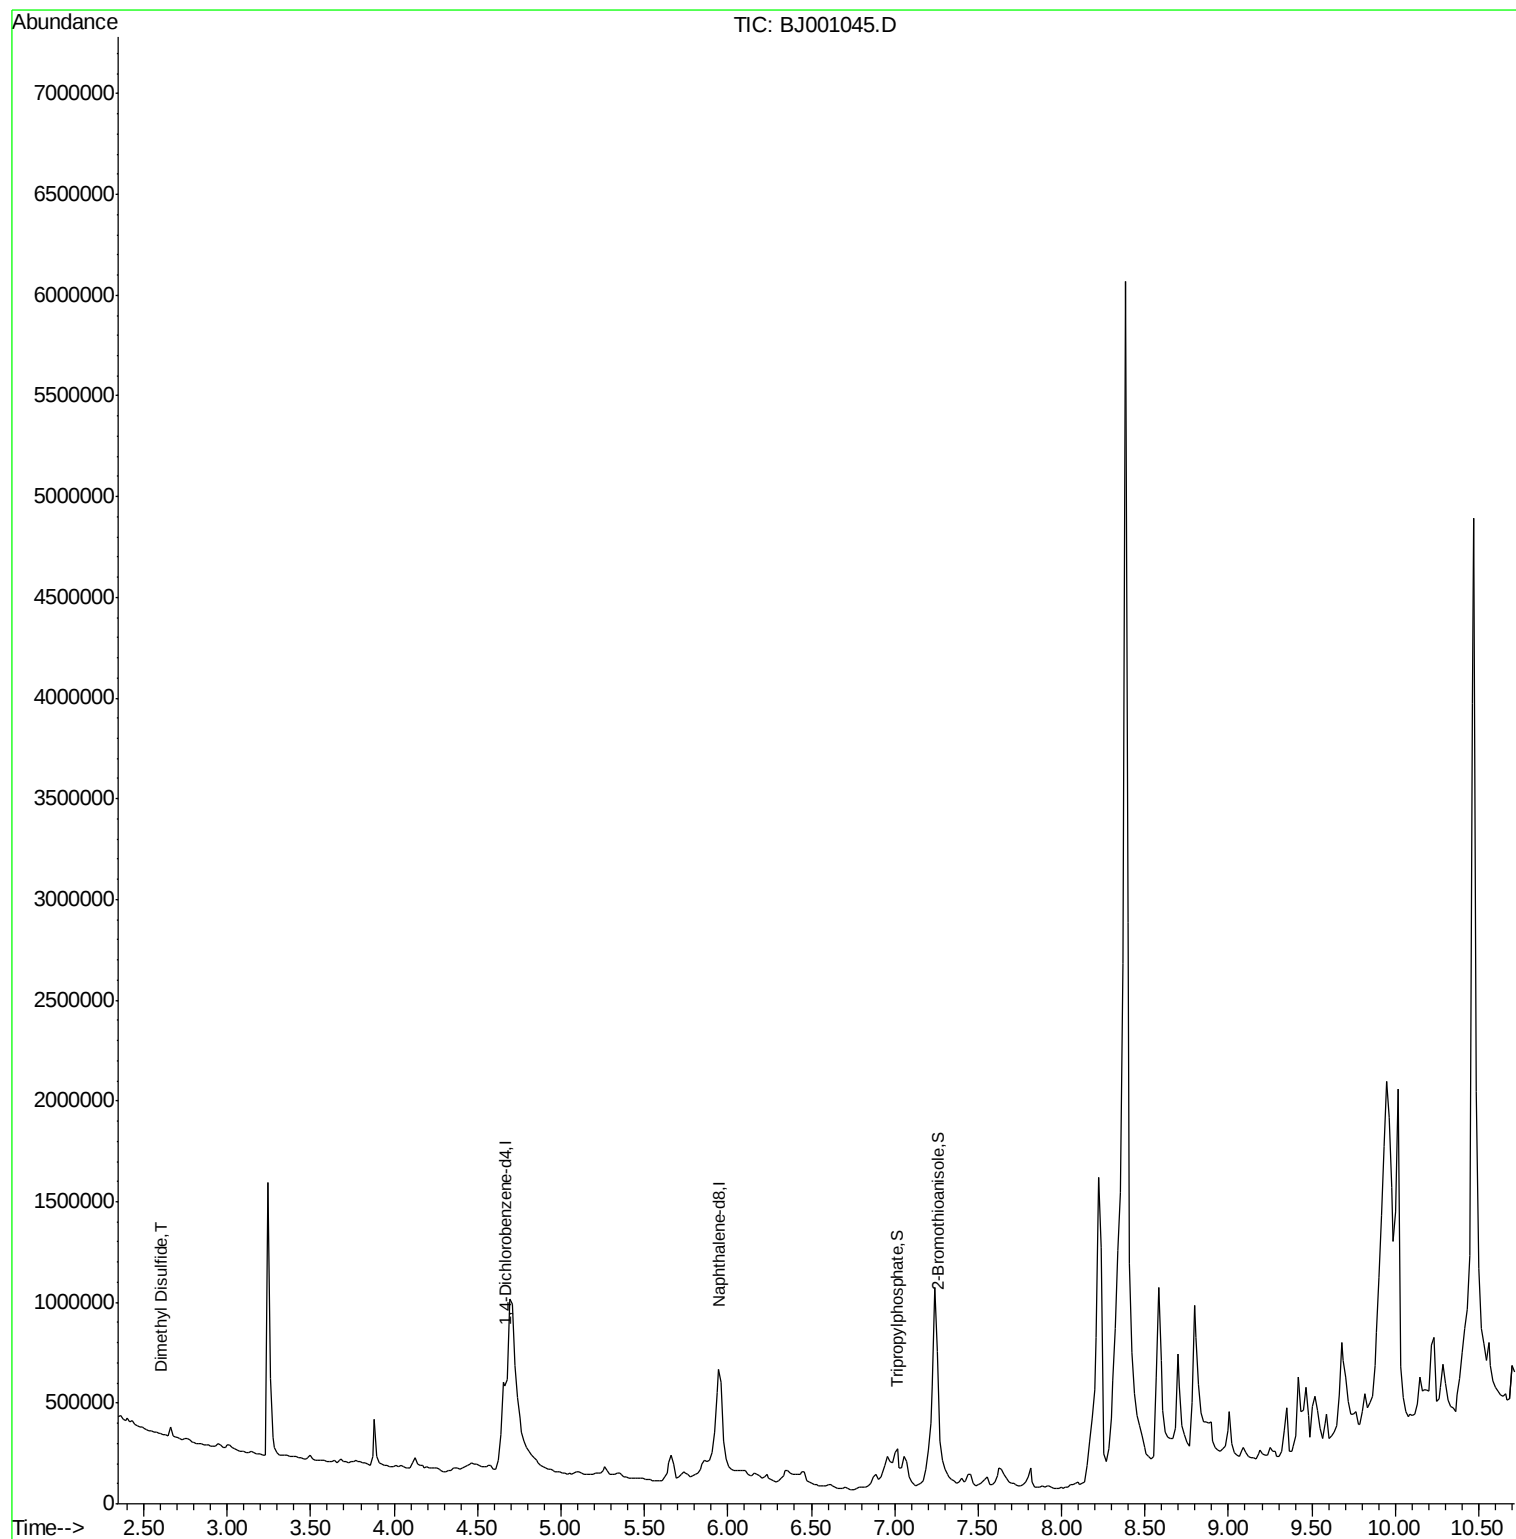


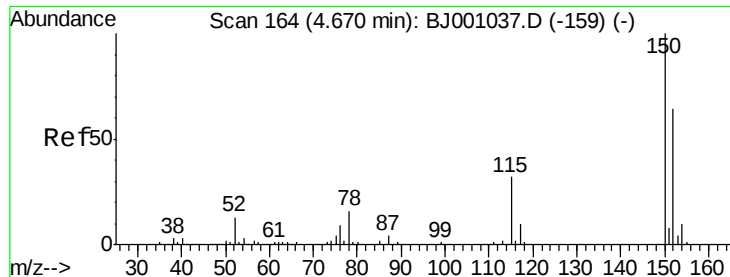




#1

1,4-Dichlorobenzene-d4
Concen: 2.00 ug/mL
RT: 4.67 min Scan# 164
Delta R.T. -0.00 min
Lab File: BJ001045.D
Acq: 20 Jul 2012 15:44

Tgt Ion: 152 Resp: 239229
Ion Ratio Lower Upper
152 100
115 49.3 29.0 69.0

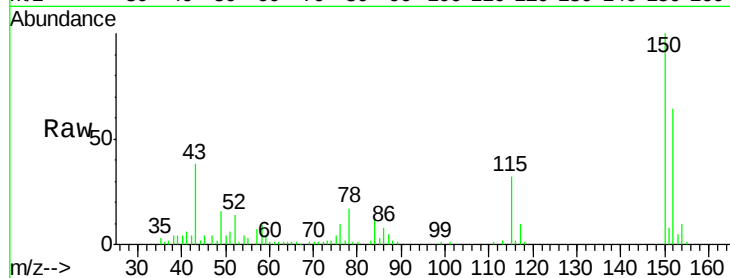


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 115.00 (114.70 to 115.70): E

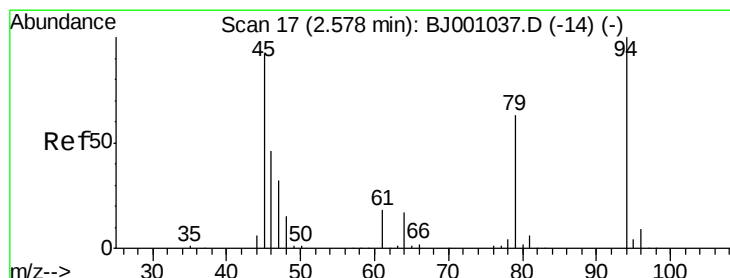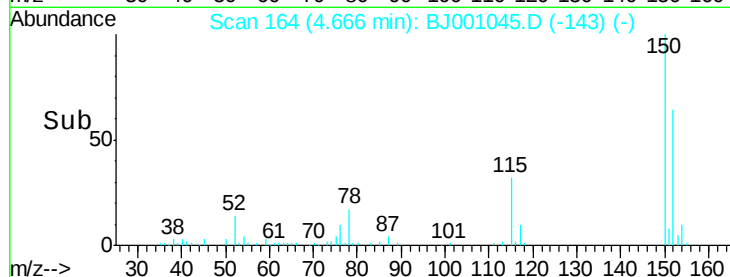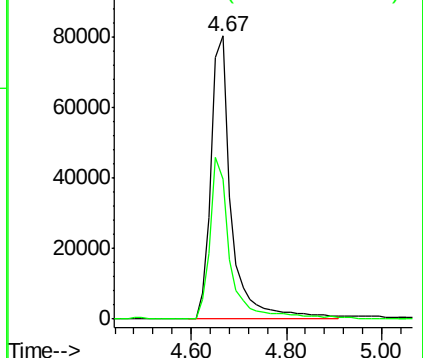



#2


Dimethyl Disulfide
Concen: 0.01 ug/mL
RT: 2.60 min Scan# 19
Delta R.T. 0.02 min
Lab File: BJ001045.D
Acq: 20 Jul 2012 15:44

Tgt Ion: 94 Resp: 640
Ion Ratio Lower Upper
94 100
45 135.1 75.2 115.2#
79 0.0 43.1 83.1#

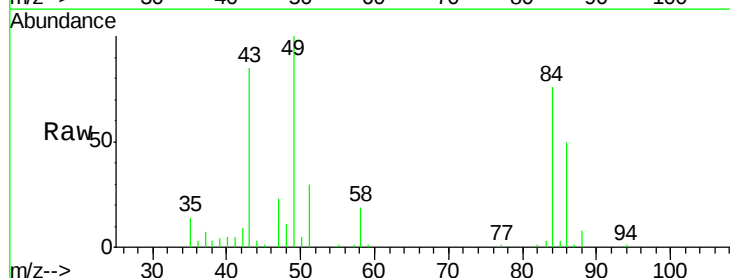

Abundance Ion 94.00 (93.70 to 94.70): BJ0
Ion 45.00 (44.70 to 45.70): BJ0
Ion 79.00 (78.70 to 79.70): BJ0

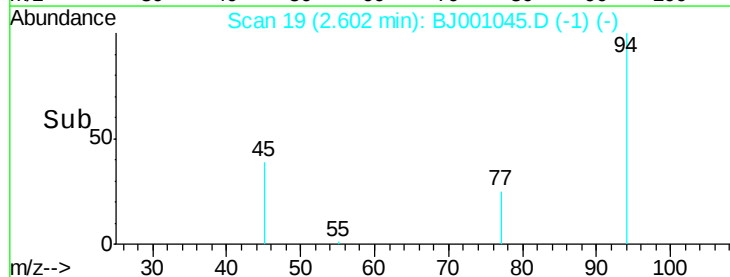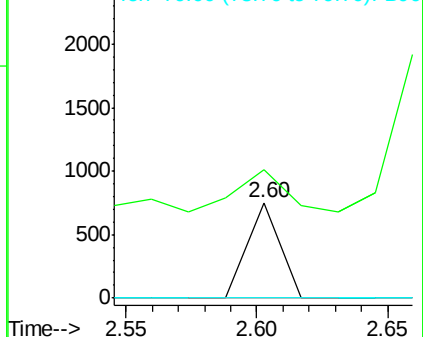

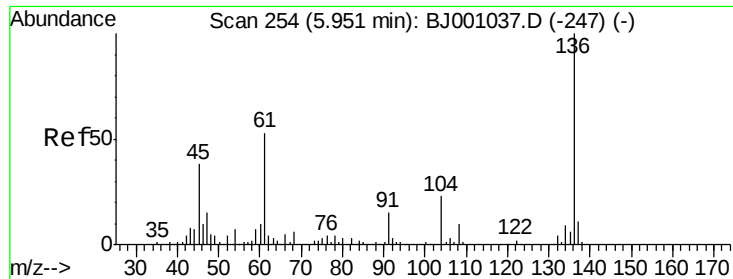

#6

Naphthalene-d8

Concen: 2.00 ug/mL

RT: 5.95 min Scan# 254

Delta R.T. -0.00 min

Lab File: BJ001045.D



Acq: 20 Jul 2012 15:44

Tgt Ion:136 Resp: 957275

Ion Ratio Lower Upper


136 100

68 6.9 0.0 25.5

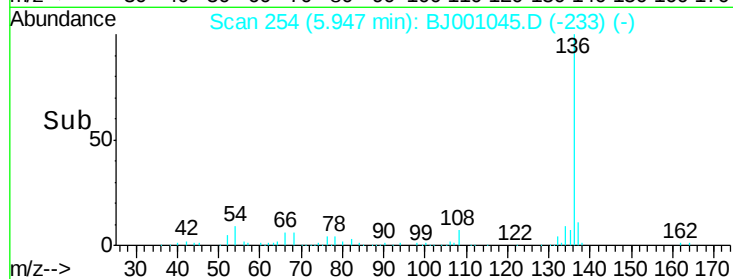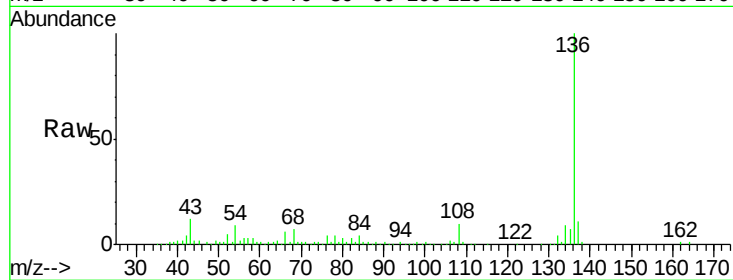

Abundance Ion 136.00 (135.70 to 136.70): E

Ion 68.00 (67.70 to 68.70): BJ0

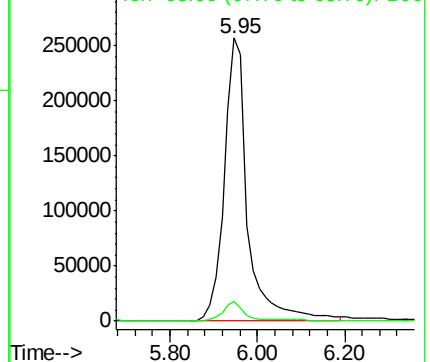

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ072012\
 Data File : BJ001045.D
 Acq On : 20 Jul 2012 15:44
 Operator : HLM
 Sample : D3359-01
 Misc : WATER BNA_J HLM
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Jul 21 05:01:09 2012
 Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ072012.M
 Quant Title : CWA degradation products by GCMS
 QLast Update : Fri Jul 20 14:08:00 2012
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.67	152	239229	2.00	ug/mL	0.00
6) Naphthalene-d8	5.95	136	957275	2.00	ug/mL	0.00

System Monitoring Compounds						
10) Tripropylphosphate	7.01	99	214200	0.61	ug/mL	0.00
Spiked Amount 0.500	Range	70 - 130	Recovery	=	122.00%	
12) 2-Bromothioanisole	7.26	204	337411	4.51	ug/mL	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	90.20%	

Target Compounds					Qvalue
2) Dimethyl Disulfide	2.60	94	640	0.01 ug/mL#	43

(#) = qualifier out of range (m) = manual integration (+) = signals summed