

DFTPP

Data File : H:\VOL1\GCMSDATA\J\120720\BJ001034.D

Vial: 1

Acq On : 20 Jul 2012 11:23

Operator: HLM

Sample : DFTPP050

Inst : BNA_J


Misc : DFTPP050 BNA_J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ072012.M (RTE Integrator)

Title : CWA degradation products by GCMS

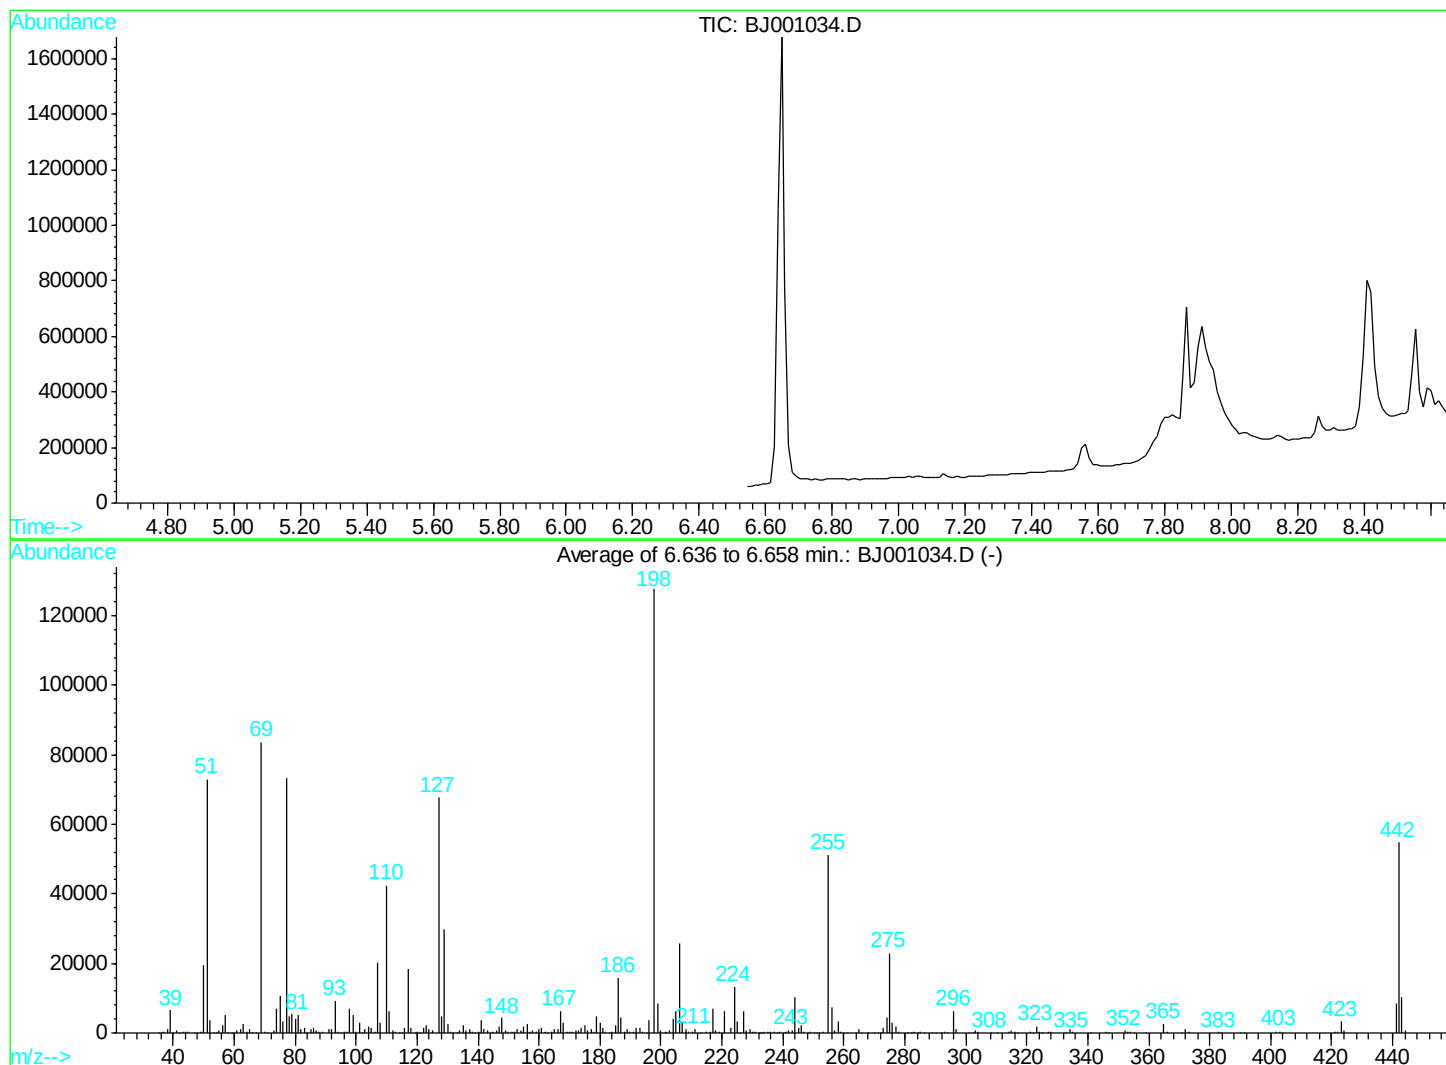

AutoFind: Scans 9, 10, 11; Background Corrected with Scan 4

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	57.2	73051	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	65.5	83588	PASS
70	69	0.00	2	0.4	363	PASS
127	198	40	60	53.0	67605	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	127608	PASS
199	198	5	9	6.7	8505	PASS
275	198	10	30	18.0	22968	PASS
365	198	1	100	2.1	2721	PASS
441	443	0.01	100	81.1	8473	PASS
442	198	40	100	42.8	54680	PASS
443	442	17	23	19.1	10452	PASS