


Data Path : Z:\HPCHEM1\BNA_J\data\BJ080112\
Data File : BJ001059.D
Acq On : 1 Aug 2012 14:01
Operator : HLM
Sample : P4-CCV
Misc : 1.0PPM BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1




Instrument :
BNA_J
ClientSampleId :
P4-CCV

Manual Integrations
APPROVED

AHPatel
8/3/2012 7:08:18 AM

Quant Time: Aug 03 01:40:17 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Aug 01 16:27:38 2012
Response via : Initial Calibration

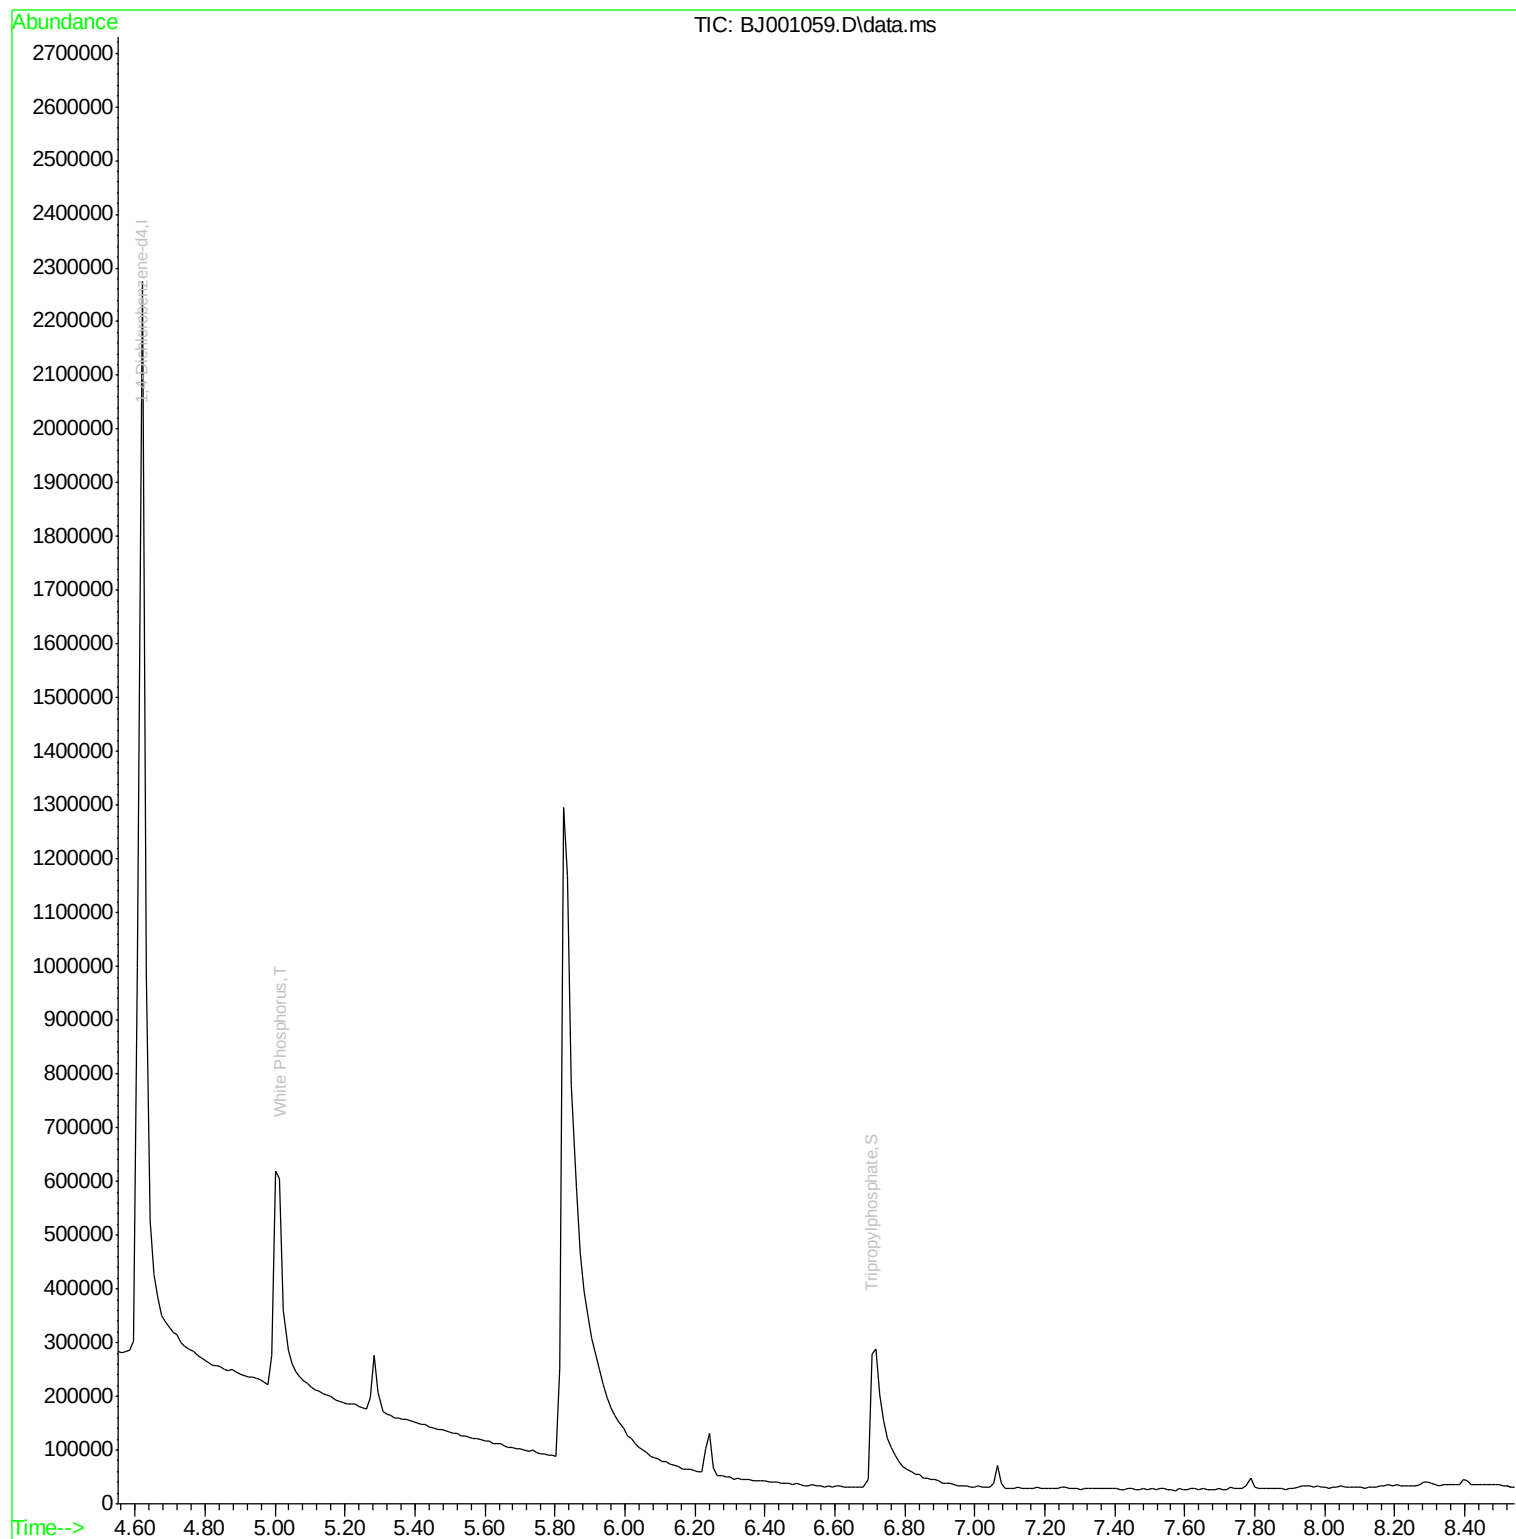

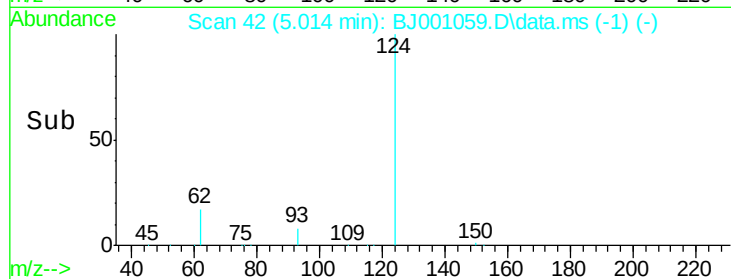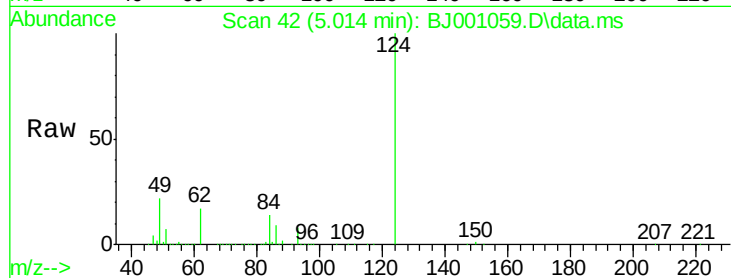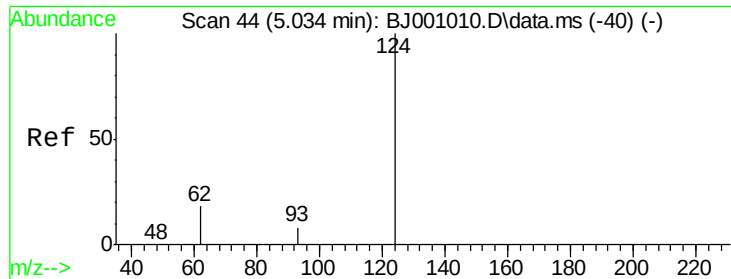

#3

White Phosphorus

Concen: 1.06 ug/ml

RT: 5.014 min Scan# 42

Delta R.T. 0.000 min

Lab File: BJ001059.D

Acq: 1 Aug 2012 14:01

Instrument :

BNA_J


ClientSampleId :

P4-CCV

Tgt Ion	Ratio	Resp Lower	Resp Upper
124	100		737365
93	8.4	0.0	28.4
62	20.6	0.6	40.6

Manual Integrations
APPROVED

AHPatel
8/3/2012 7:08:18 AM

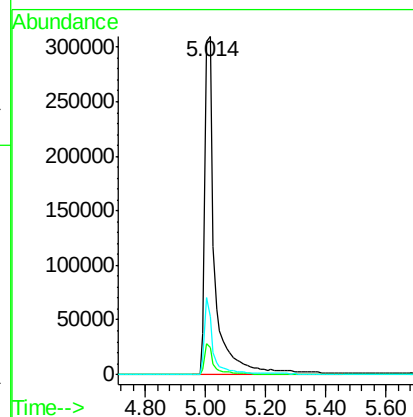

Data Path : Z:\HPCHEM1\BNA_J\data\BJ080112\
Data File : BJ001059.D
Acq On : 1 Aug 2012 14:01
Operator : HLM
Sample : P4-CCV
Misc : 1.0PPM BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-CCV

Manual Integrations
APPROVED

AHPatel
8/3/2012 7:08:18 AM

Quant Time: Aug 03 01:40:17 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ071812.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Aug 01 16:27:38 2012
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	4.620	150	841514	2.50	ug/ml	0.00
System Monitoring Compounds						
2) Tripropylphosphate	6.705	99	564354m	0.84	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	33.60%
Target Compounds						
3) White Phosphorus	5.014	124	737365	1.06	ug/ml	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed