


Data Path : Z:\HPCHEM1\BNA_J\data\BJ080112\
 Data File : BJ001058.D
 Acq On : 1 Aug 2012 13:42
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_J\method\BJ071812.M
 Title : P4 by SOP M.5
 Last Update : Wed Jul 18 14:02:57 2012

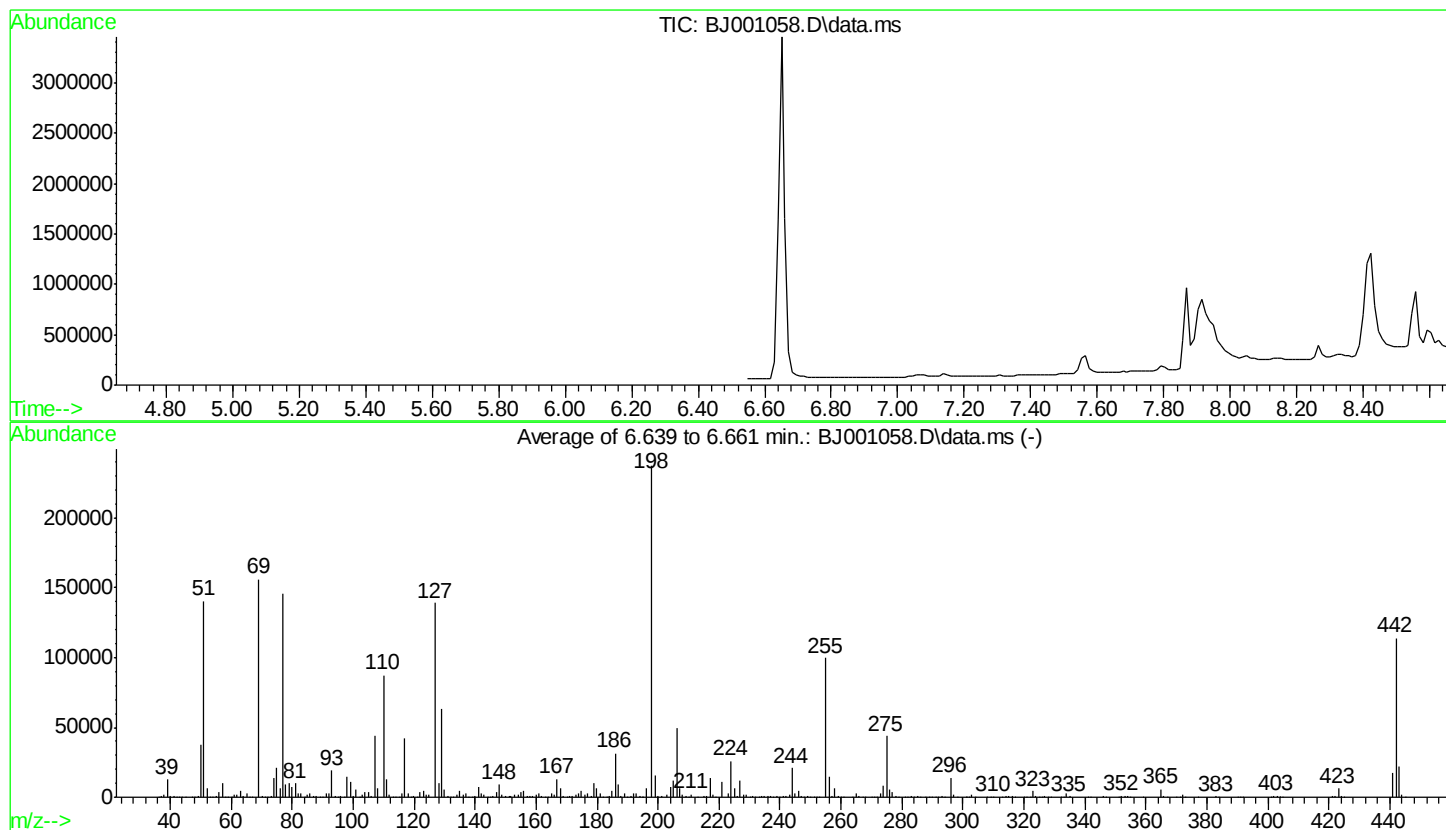

AutoFind: Scans 9, 10, 11; Background Corrected with Scan 4

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	59.2	140602	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	65.7	156140	PASS
70	69	0.00	2	0.4	650	PASS
127	198	40	60	58.5	139035	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	237546	PASS
199	198	5	9	6.6	15717	PASS
275	198	10	30	18.4	43634	PASS
365	198	1	100	2.4	5627	PASS
441	443	0.01	100	76.8	17028	PASS
442	198	40	100	48.0	114077	PASS
443	442	17	23	19.4	22169	PASS