


Data Path : S:\HPCHEM1\BNA_J\data\BJ081612\
 Data File : BJ001074.D
 Acq On : 16 Aug 2012 13:19
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : S:\HPCHEM1\BNA_J\method\BJ072012.M
 Title : CWA degradation products by GCMS
 Last Update : Fri Jul 20 14:09:12 2012

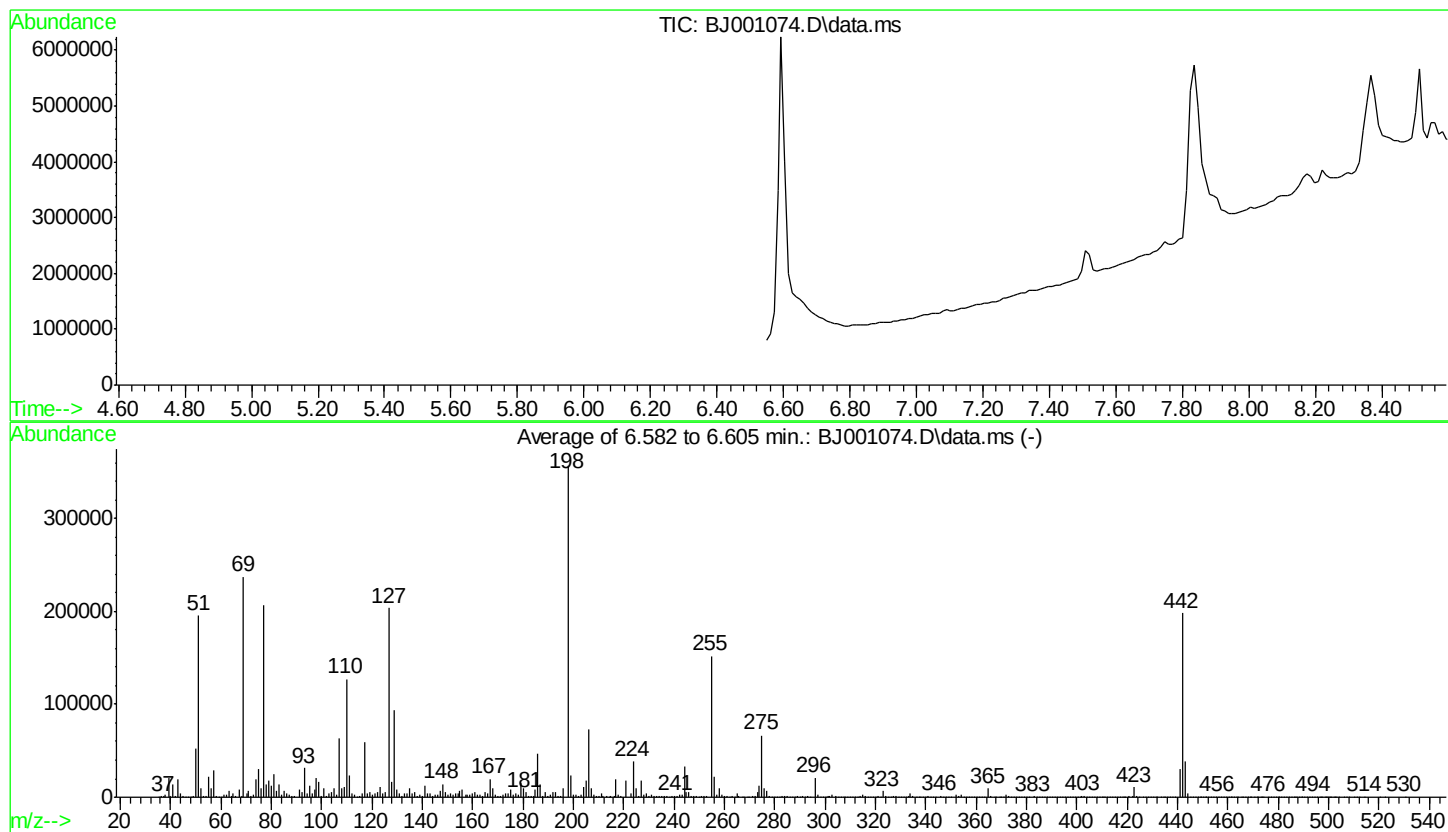

AutoFind: Scans 4, 5, 6; Background Corrected with Scan 2

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	54.6	194992	PASS
68	69	0.00	2	0.5	1074	PASS
69	198	0.00	100	66.5	237400	PASS
70	69	0.00	2	1.7	3967	PASS
127	198	40	60	57.1	203877	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	356903	PASS
199	198	5	9	6.7	24090	PASS
275	198	10	30	18.6	66254	PASS
365	198	1	100	2.6	9267	PASS
441	443	0.01	100	77.9	30019	PASS
442	198	40	100	55.5	197968	PASS
443	442	17	23	19.5	38556	PASS