


Data Path : S:\HPCHEM1\BNA_J\data\BJ092412\
 Data File : BJ001142.D
 Acq On : 24 Sep 2012 14:27
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : S:\HPCHEM1\BNA_J\method\BJ092412.M
 Title : CWA degradation products by GCMS
 Last Update : Wed Oct 03 18:08:32 2012

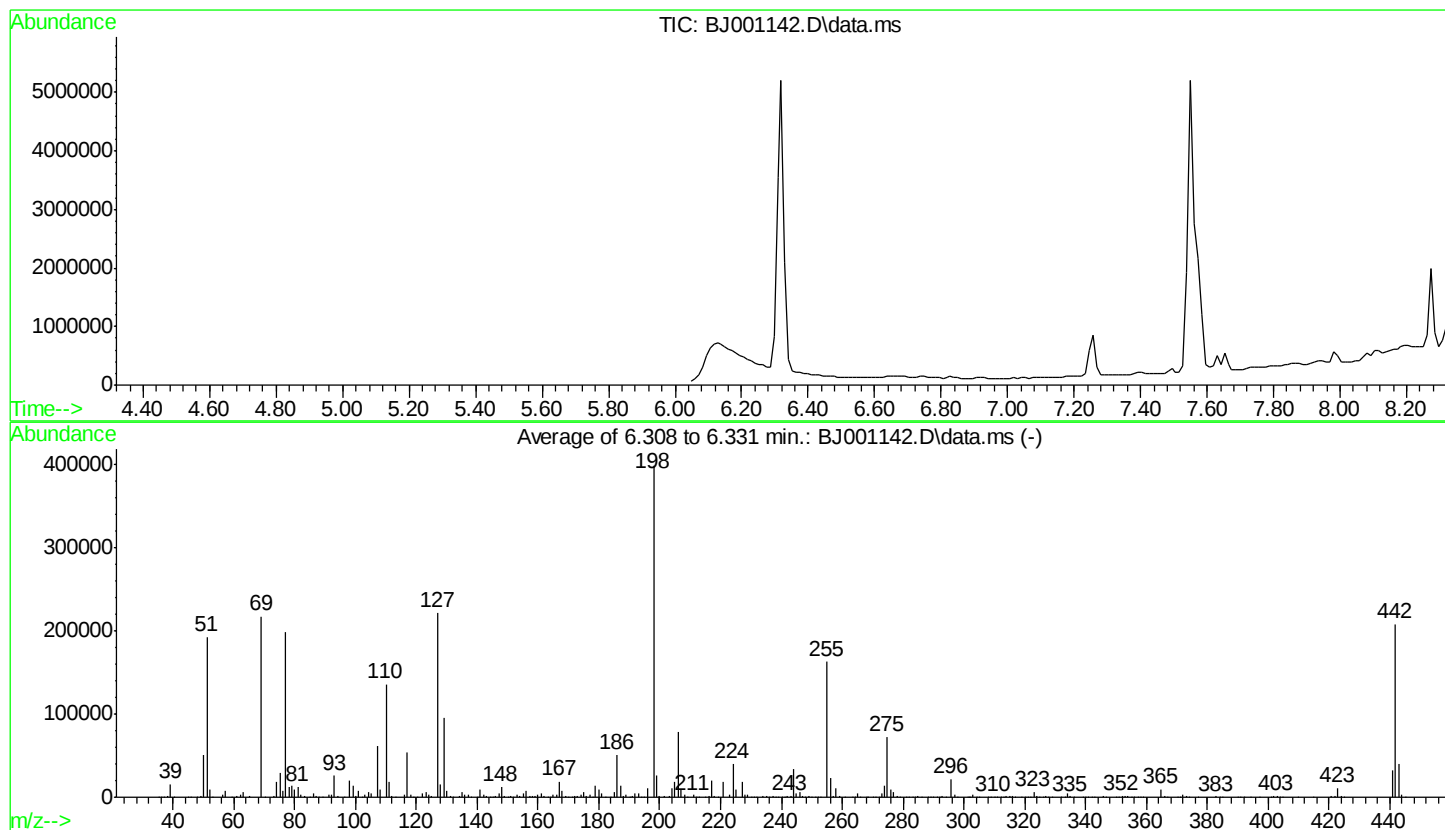

AutoFind: Scans 24, 25, 26; Background Corrected with Scan 18

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	48.4	193024	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	54.6	217628	PASS
70	69	0.00	2	0.1	204	PASS
127	198	40	60	55.7	221755	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	398459	PASS
199	198	5	9	6.6	26281	PASS
275	198	10	30	18.3	72741	PASS
365	198	1	100	2.4	9417	PASS
441	443	0.01	100	80.6	32069	PASS
442	198	40	100	52.3	208405	PASS
443	442	17	23	19.1	39789	PASS