


Data Path : S:\HPCHEM1\BNA_J\data\BJ100312\
 Data File : BJ001153.D
 Acq On : 3 Oct 2012 12:47
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : S:\HPCHEM1\BNA_J\method\BJ092412.M
 Title : CWA degradation products by GCMS
 Last Update : Wed Oct 03 18:08:32 2012

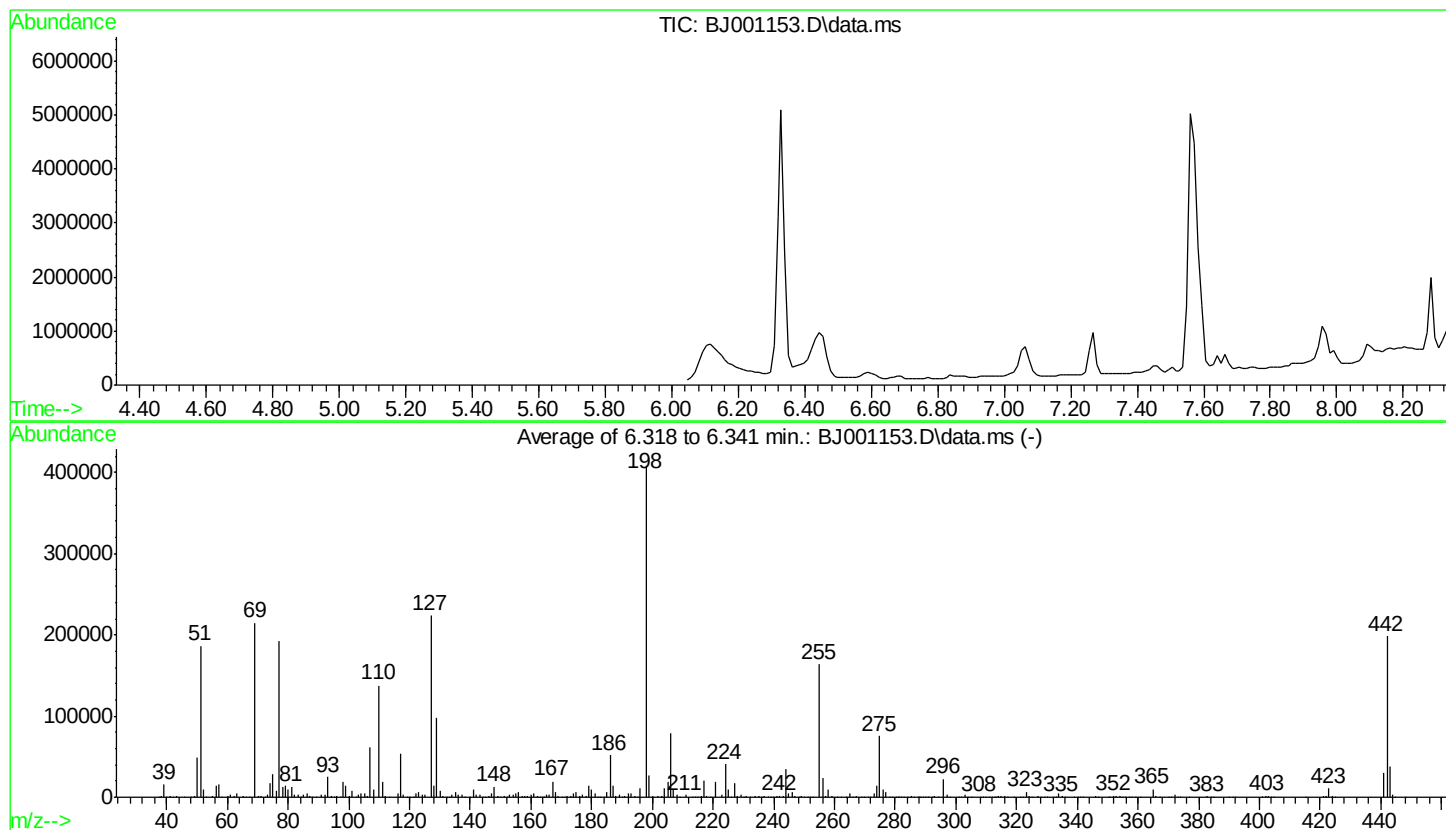

AutoFind: Scans 25, 26, 27; Background Corrected with Scan 18

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	45.6	186388	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.6	215090	PASS
70	69	0.00	2	0.5	1025	PASS
127	198	40	60	54.7	223486	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	408529	PASS
199	198	5	9	6.5	26662	PASS
275	198	10	30	18.4	75094	PASS
365	198	1	100	2.4	9622	PASS
441	443	0.01	100	78.4	29983	PASS
442	198	40	100	48.6	198437	PASS
443	442	17	23	19.3	38266	PASS