

Data File : H:\VOL1\GCMSDATA\J\121004\BJ001172.D
Acq On : 4 Oct 2012 16:13
Sample : P4-1
Misc : BNA_J HLM
MS Integration Params: RTEINT.P
Quant Time: Oct 4 17:42 2012

Vial: 8
Operator: HLM
Inst : BNA_J
Multiplr: 1.00

Instrument :
BNA_J
LabSampleId :
P4-1

Quant Results File: BJ100412.FRES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M (RTE Integrator)
Title : P4 by SOP M.5
Last Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration
DataAcq Meth : P4

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	150	1369587	2.50	ug/ml	0.00
System Monitoring Compounds						
2) Tripropylphosphate	6.47	99	133768	0.12	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	4.80%#
Target Compounds						
3) White Phosphorus	4.74	124	133354	0.11	ug/ml	Ovalue 100

Data File : H:\VOL1\GCMSDATA\J\121004\BJ001172.D

Vial: 8

Acq On : 4 Oct 2012 16:13

Operator: HLM

Sample : P4-1

Inst : BNA J

Misc : BNA_J HLM

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Oct 4 17:42 2012

Quant Results File: BJ100412.P

Instrument :

BNA_J

LabSampleId :


P4-1


Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M (RTE Integrator)

Title : P4 by SOP M.5

Last Update : Thu Oct 04 17:38:53 2012

Response via : Initial Calibration

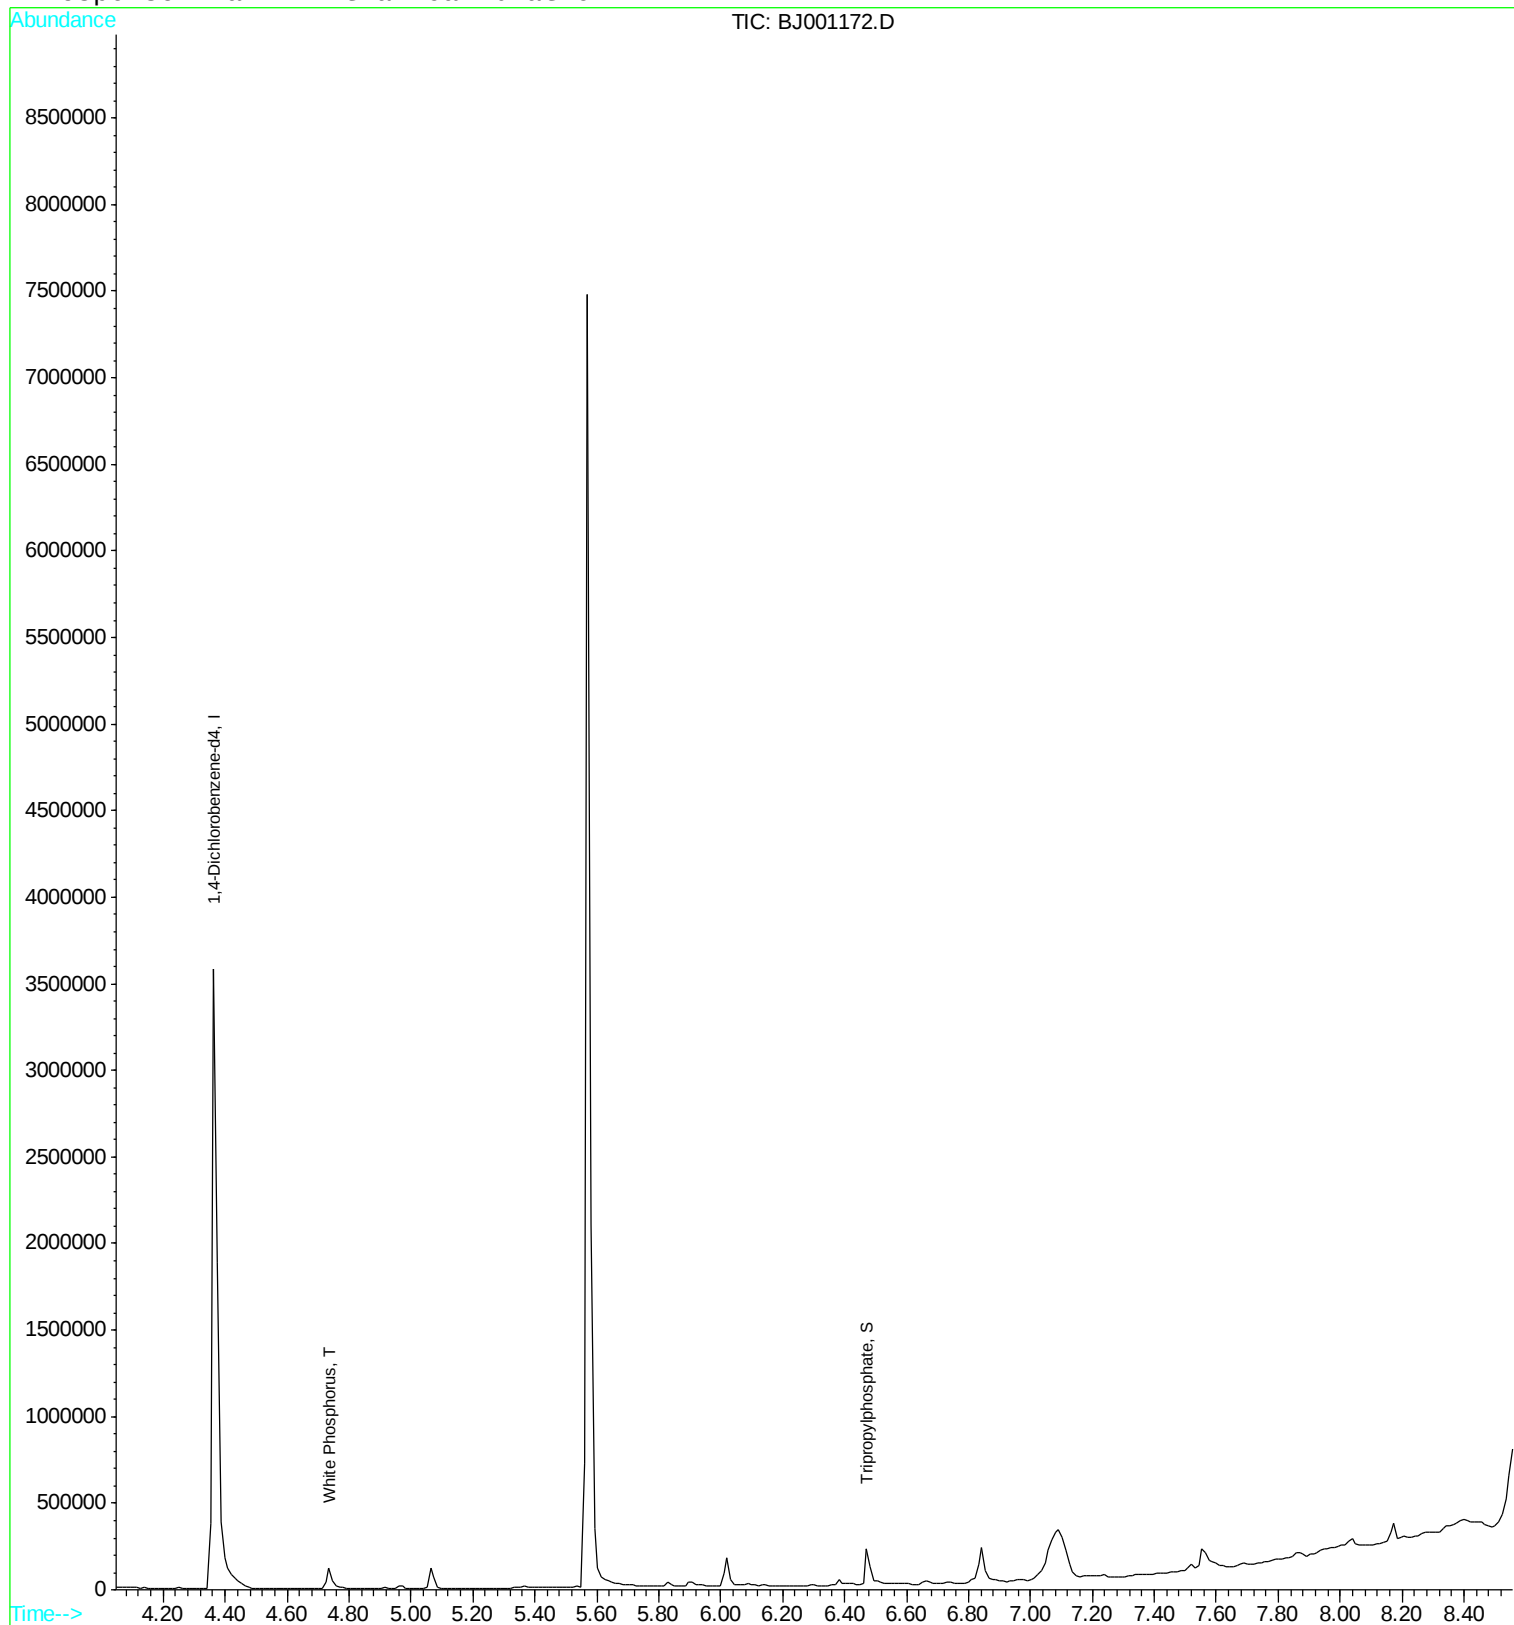

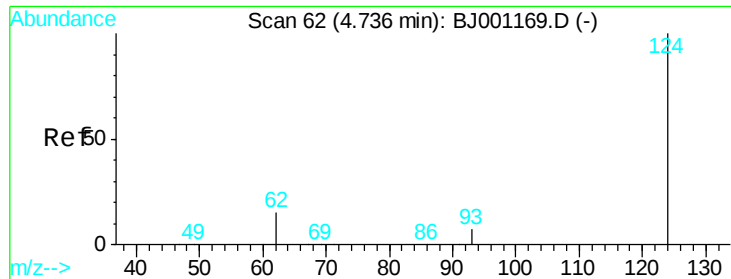

#3

White Phosphorus

Concen: 0.11 ug/ml

RT: 4.74 min Scan# 62

Delta R.T. -0.00 min

Lab File: BJ001172.D


Acq: 4 Oct 2012 16:13

Instrument :

BNA_J

LabSampleId :

P4-1

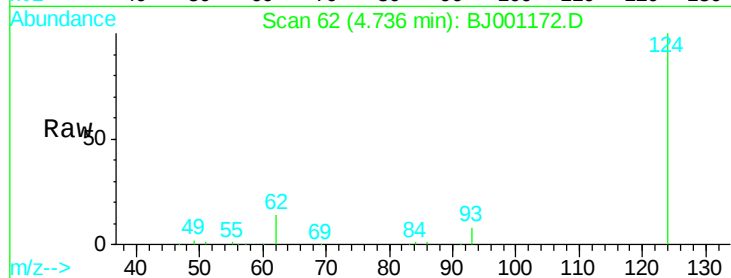

Tgt Ion:	124	Resp:	133354
Ion	Ratio	Lower	Upper
124	100		
93	7.6	0.0	27.3
62	15.7	0.0	35.7

