

Data File : H:\VOL1\GCMSDATA\J\121004\BJ001173.D
Acq On : 4 Oct 2012 16:26
Sample : P4-ICV
Misc : BNA_J HLM
MS Integration Params: RTEINT.P
Quant Time: Oct 4 17:49 2012

Vial: 9
Operator: HLM
Inst : BNA_J
Multiplr: 1.00

Instrument :
BNA_J
ClientSampleId :
P4-ICV

Quant Results File: BJ100412.M

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M (RTE Integrator)
Title : P4 by SOP M.5
Last Update : Thu Oct 04 17:45:25 2012
Response via : Initial Calibration
DataAcq Meth : P4

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	150	973970	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	0.00	99	0	0.00	ug/ml	
Spiked Amount	2.500	Range	20 - 150	Recovery	=	0.00%#

Target Compounds

3) White Phosphorus	4.74	124	861130	0.94	ug/ml	Ovalue 99
---------------------	------	-----	--------	------	-------	--------------

Data File : H:\VOL1\GCMSDATA\J\121004\BJ001173.D

Vial: 9

Acq On : 4 Oct 2012 16:26

Operator: HLM

Sample : P4-ICV

Inst : BNA J

Misc : BNA_J HLM

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Oct 4 17:49 2012

Quant Results File: BJ100412.P

Instrument :

BNA_J

ClientSampleId :


P4-ICV


Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M (RTE Integrator)

Title : P4 by SOP M.5

Last Update : Thu Oct 04 17:46:22 2012

Response via : Initial Calibration

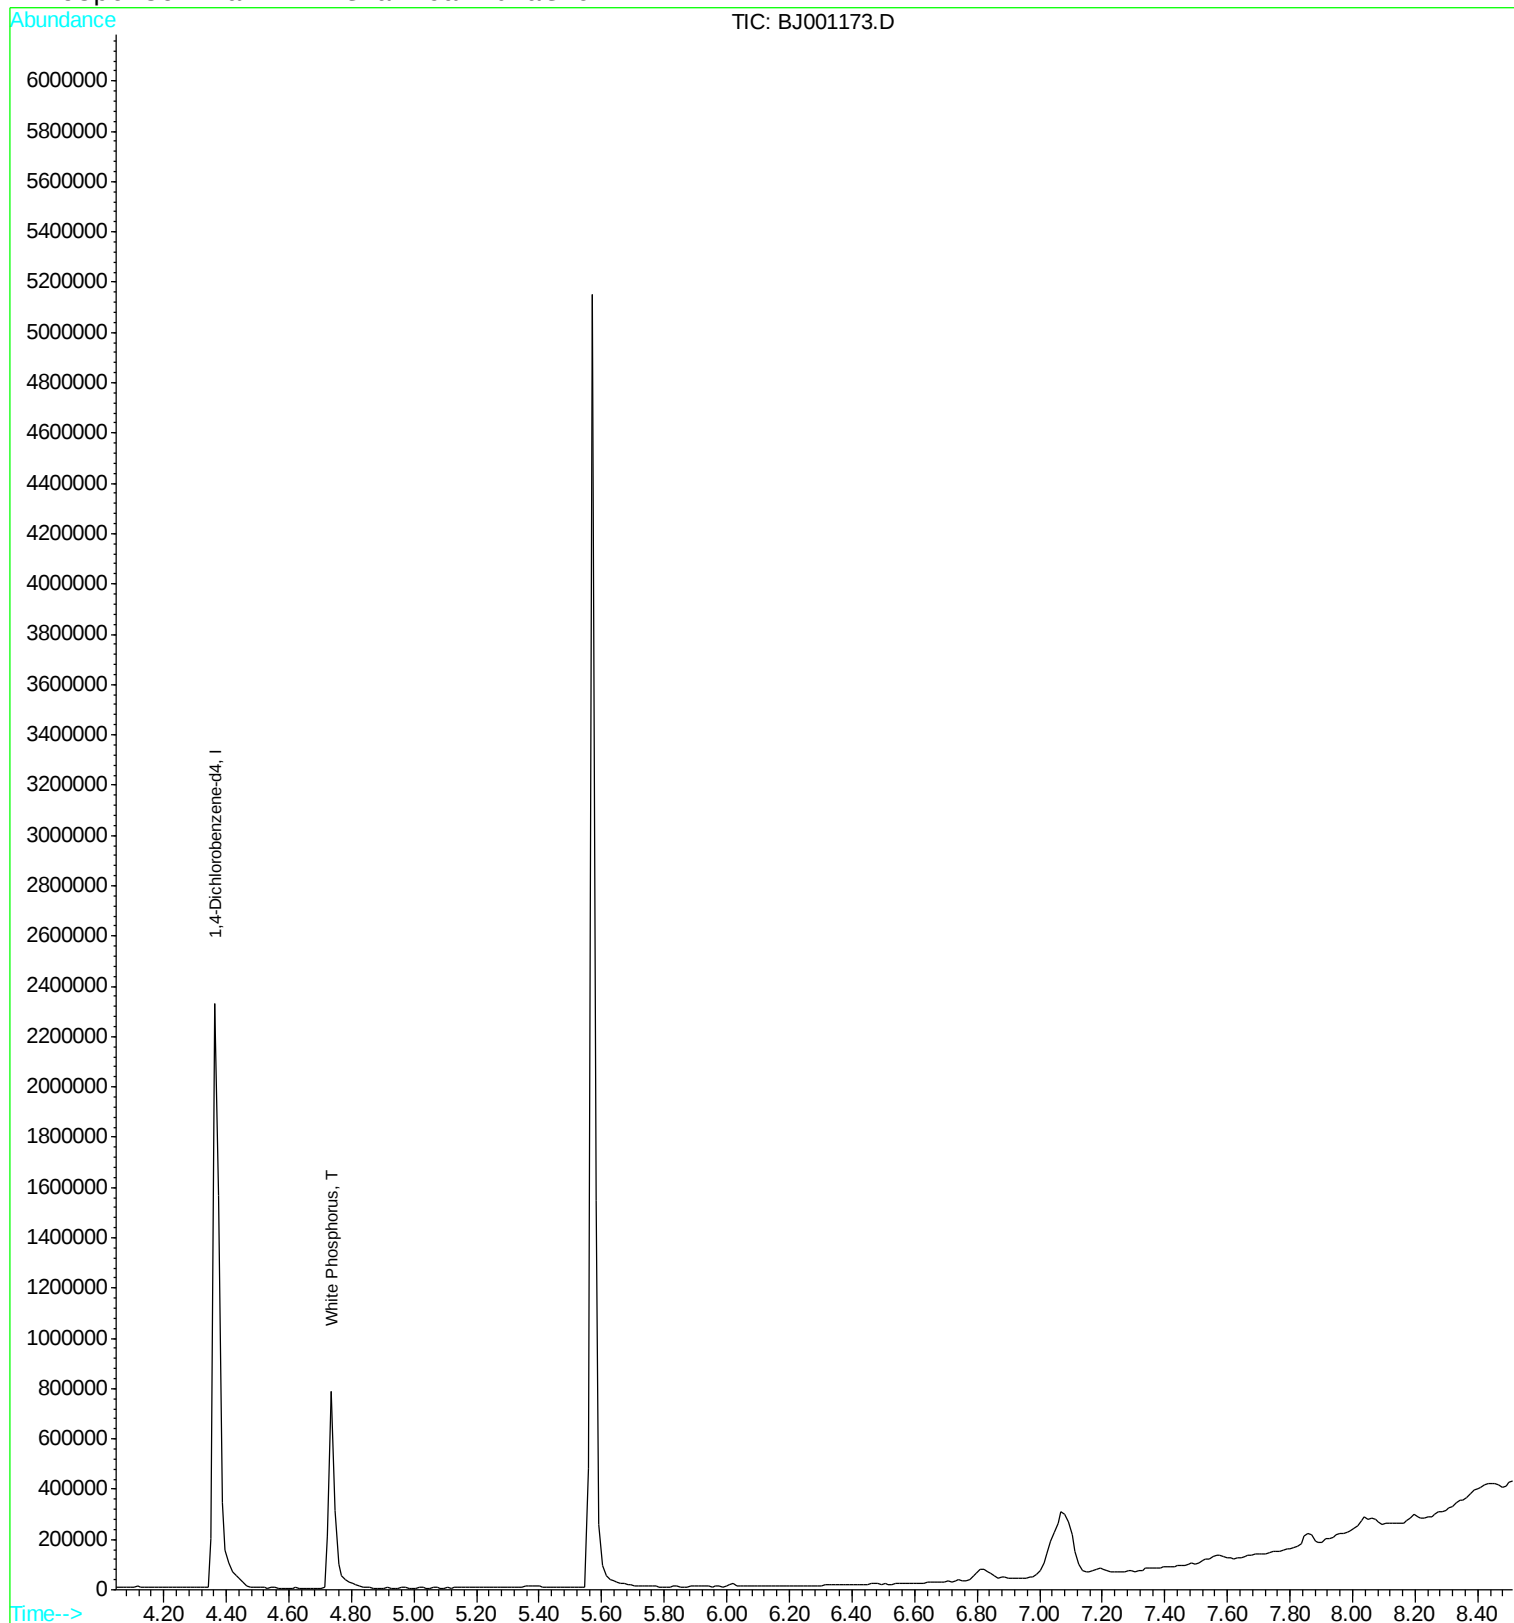

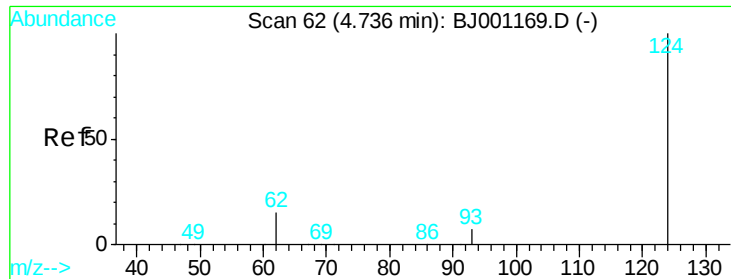

#3

White Phosphorus

Concen: 0.94 ug/ml

RT: 4.74 min Scan# 62

Delta R.T. -0.00 min

Lab File: BJ001173.D


Acq: 4 Oct 2012 16:26

Instrument :

BNA_J

ClientSampleId :

P4-ICV

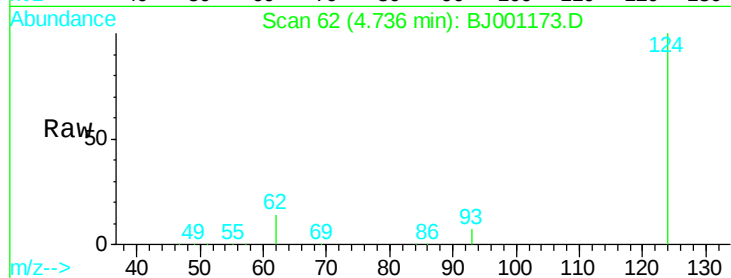


Tgt Ion:124 Resp: 861130

Ion Ratio Lower Upper

124 100

93 7.2 0.0 27.3

62 15.3 0.0 35.7

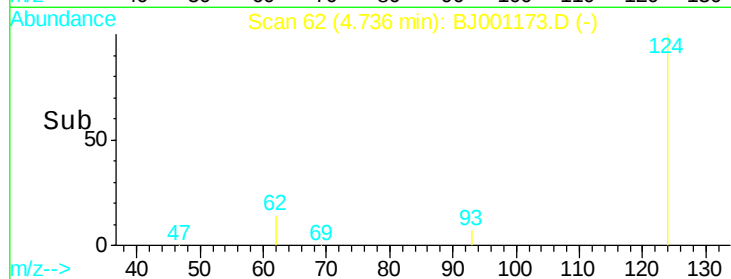

Abundance

Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

