

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001166.D
Acq On : 4 Oct 2012 14:54
Operator : HLM
Sample : P4-7
Misc : BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-7

Quant Time: Oct 06 08:24:54 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.37	150	1011486	2.50	ug/ml	0.01

System Monitoring Compounds

2) Tripropylphosphate	6.48	99	6695664	8.26	ug/ml	0.01
Spiked Amount	2.500	Range	20 - 150	Recovery	=	330.40%#


Target Compounds					Qvalue
3) White Phosphorus	4.75	124	9188934	10.52	ug/ml 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001166.D
Acq On : 4 Oct 2012 14:54
Operator : HLM
Sample : P4-7
Misc : BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-7

Quant Time: Oct 06 08:24:54 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration

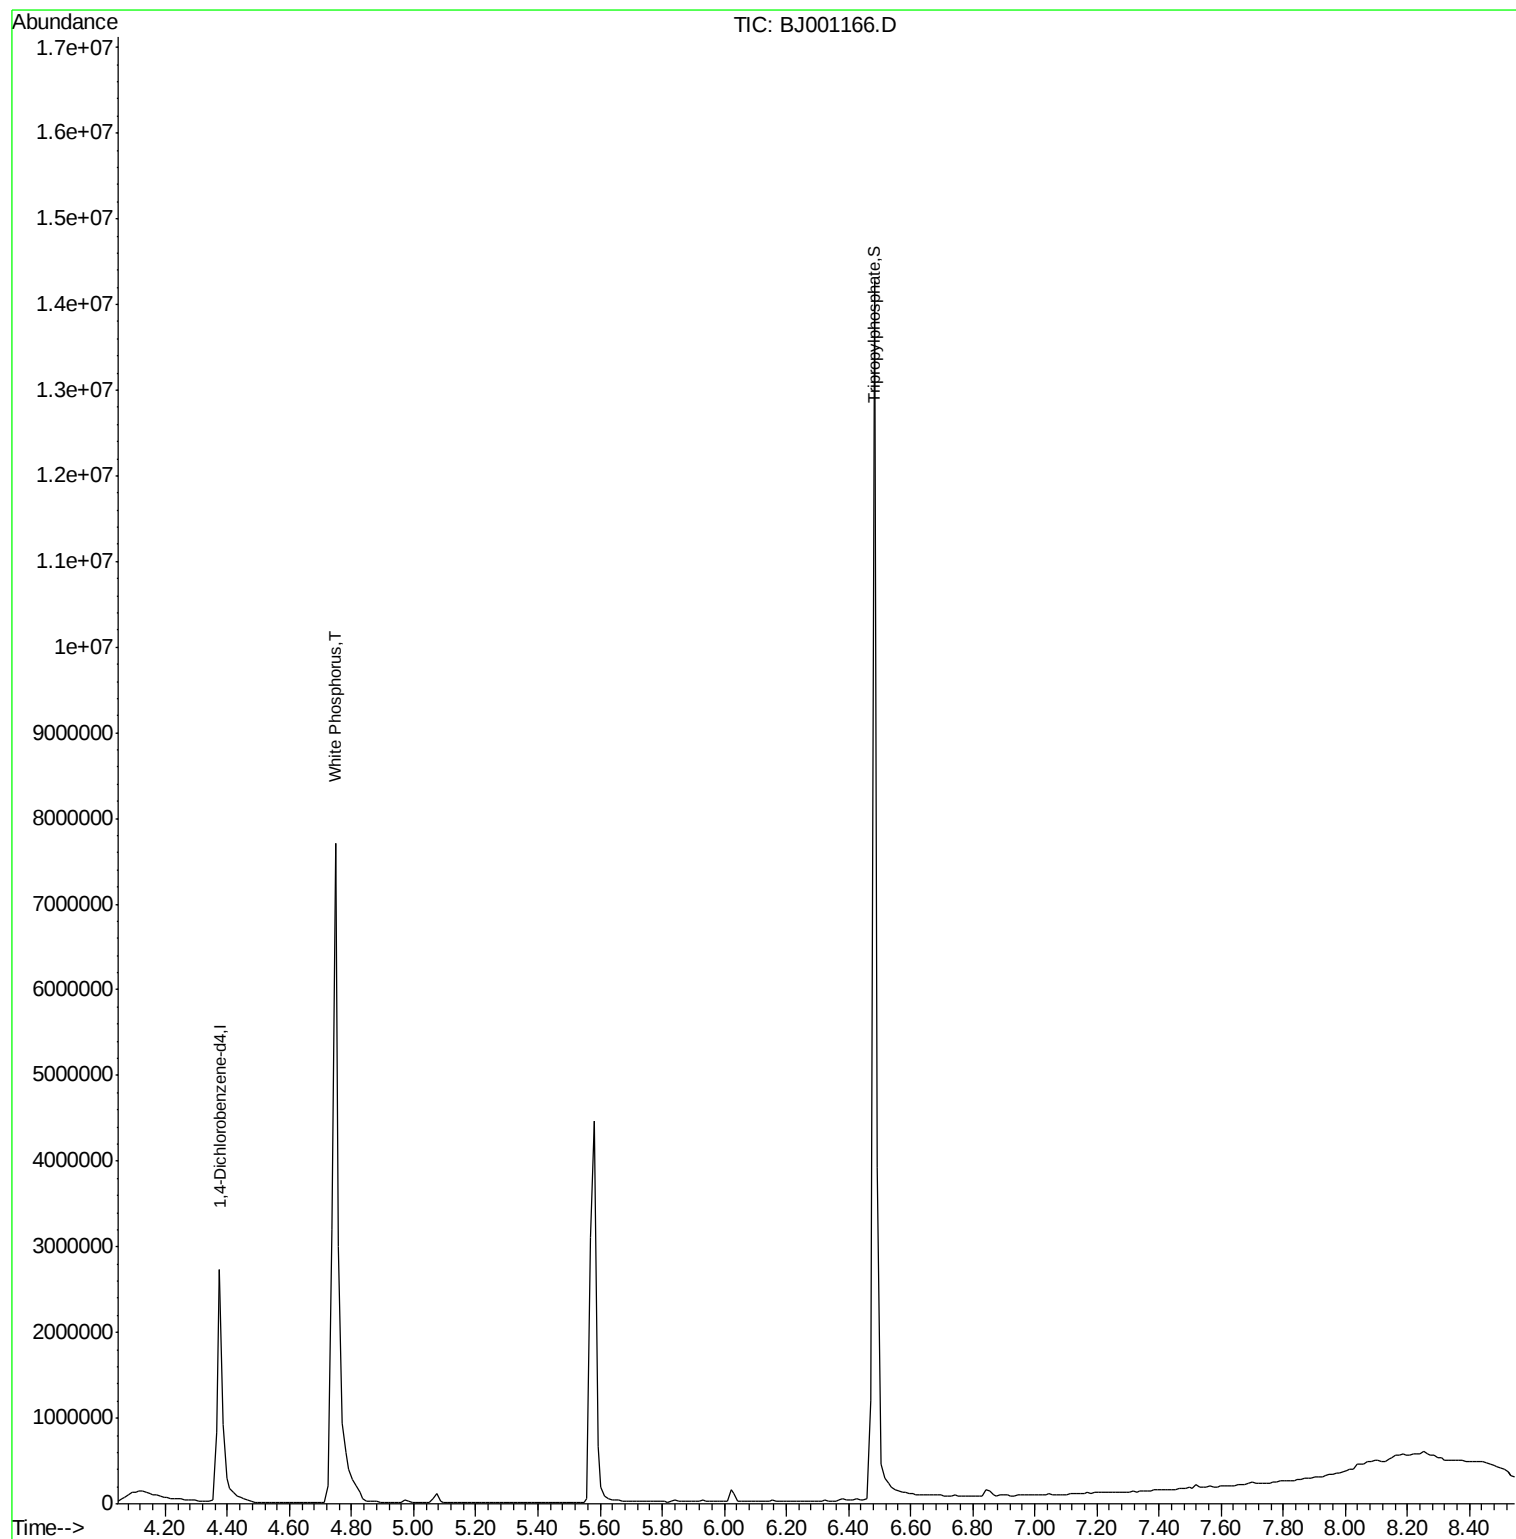


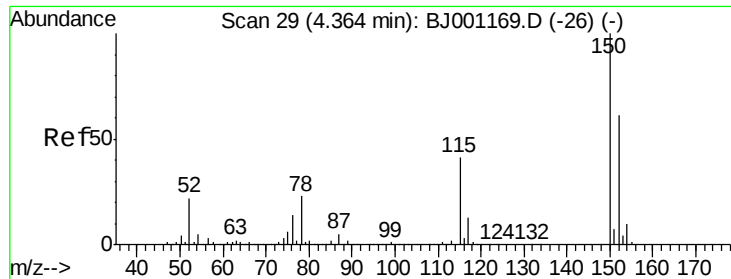




#1
 1,4-Dichlorobenzene-d4
 Concen: 2.50 ug/ml
 RT: 4.37 min Scan# 30
 Delta R.T. 0.01 min
 Lab File: BJ001166.D
 Acq: 4 Oct 2012 14:54

Instrument :
 BNA_J
 LabSampleId :
 P4-7

Tgt Ion:150 Resp: 1011486
 Ion Ratio Lower Upper
 150 100
 152 63.3 42.4 82.4

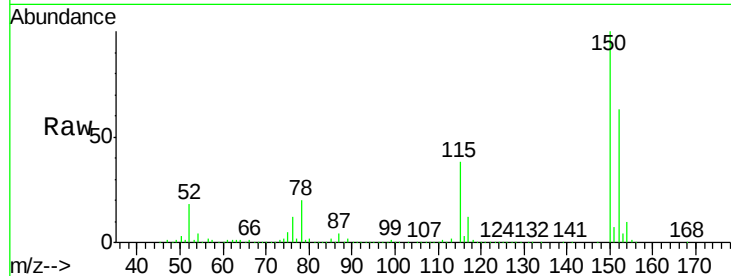


Abundance Ion 150.00 (149.70 to 150.70): E
 Ion 152.00 (151.70 to 152.70): E

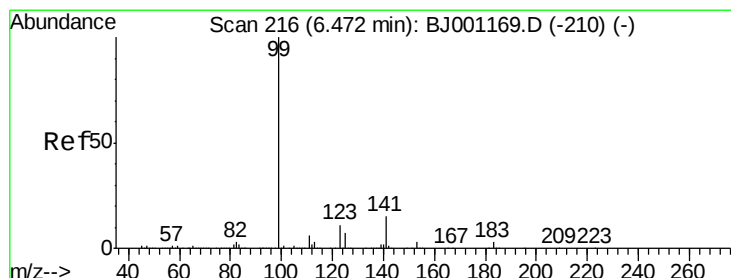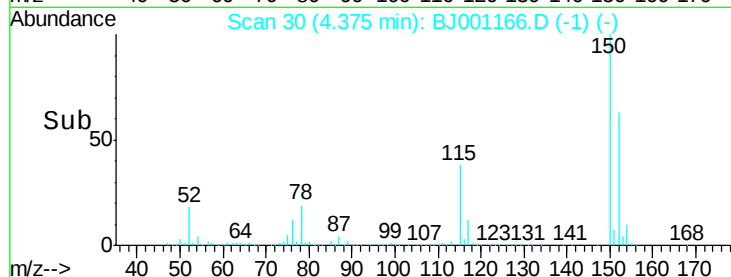
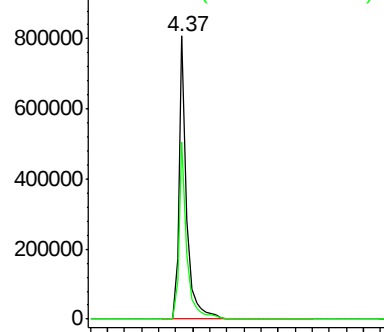



#2
 Tripropylphosphate
 Concen: 8.26 ug/ml
 RT: 6.48 min Scan# 217
 Delta R.T. 0.01 min
 Lab File: BJ001166.D
 Acq: 4 Oct 2012 14:54

Tgt Ion: 99 Resp: 6695664
 Ion Ratio Lower Upper
 99 100
 141 27.2 0.0 39.9

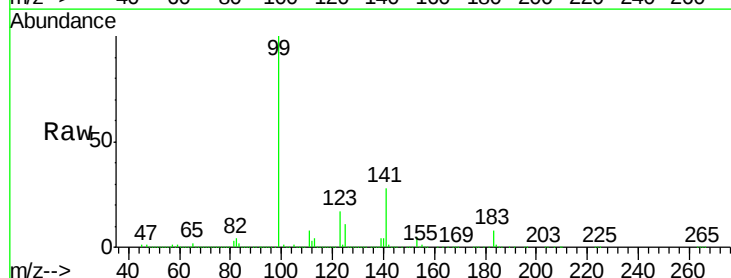

Abundance Ion 99.00 (98.70 to 99.70): BJ0
 Ion 141.00 (140.70 to 141.70): E

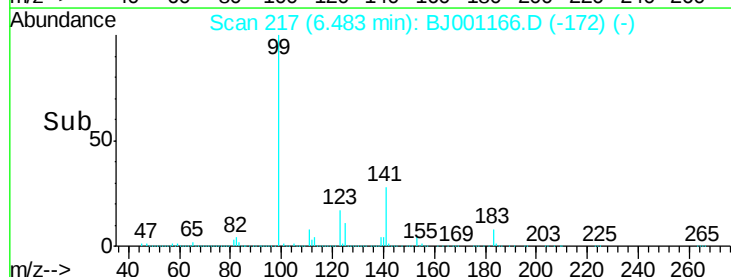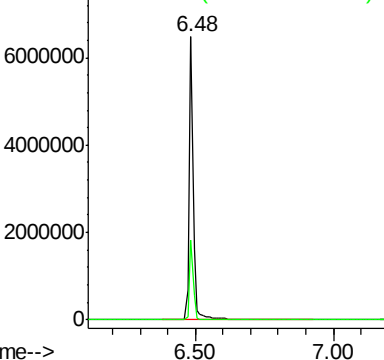

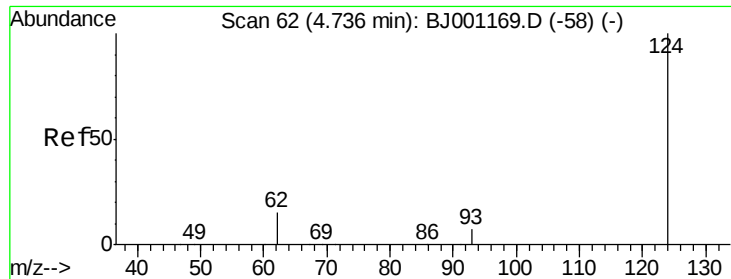

#3
 White Phosphorus
 Concen: 10.52 ug/ml
 RT: 4.75 min Scan# 63
 Delta R.T. 0.01 min
 Lab File: BJ001166.D
 Acq: 4 Oct 2012 14:54

Instrument :
 BNA_J
 LabSampleId :
 P4-7

Tgt Ion:124 Resp: 9188934
 Ion Ratio Lower Upper
 124 100
 93 7.4 0.0 27.3
 62 15.9 0.0 35.7

