

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001167.D
Acq On : 4 Oct 2012 15:07
Operator : HLM
Sample : P4-6
Misc : BNA_J HLM
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-6

Quant Time: Oct 06 08:24:56 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	150	1041933	2.50	ug/ml	0.00

System Monitoring Compounds
2) Tripropylphosphate 6.47 99 4269718 5.11 ug/ml 0.00
Spiked Amount 2.500 Range 20 - 150 Recovery = 204.40%#


Target Compounds					Qvalue
3) White Phosphorus	4.74	124	4852999	5.39 ug/ml	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001167.D
Acq On : 4 Oct 2012 15:07
Operator : HLM
Sample : P4-6
Misc : BNA_J HLM
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-6

Quant Time: Oct 06 08:24:56 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration

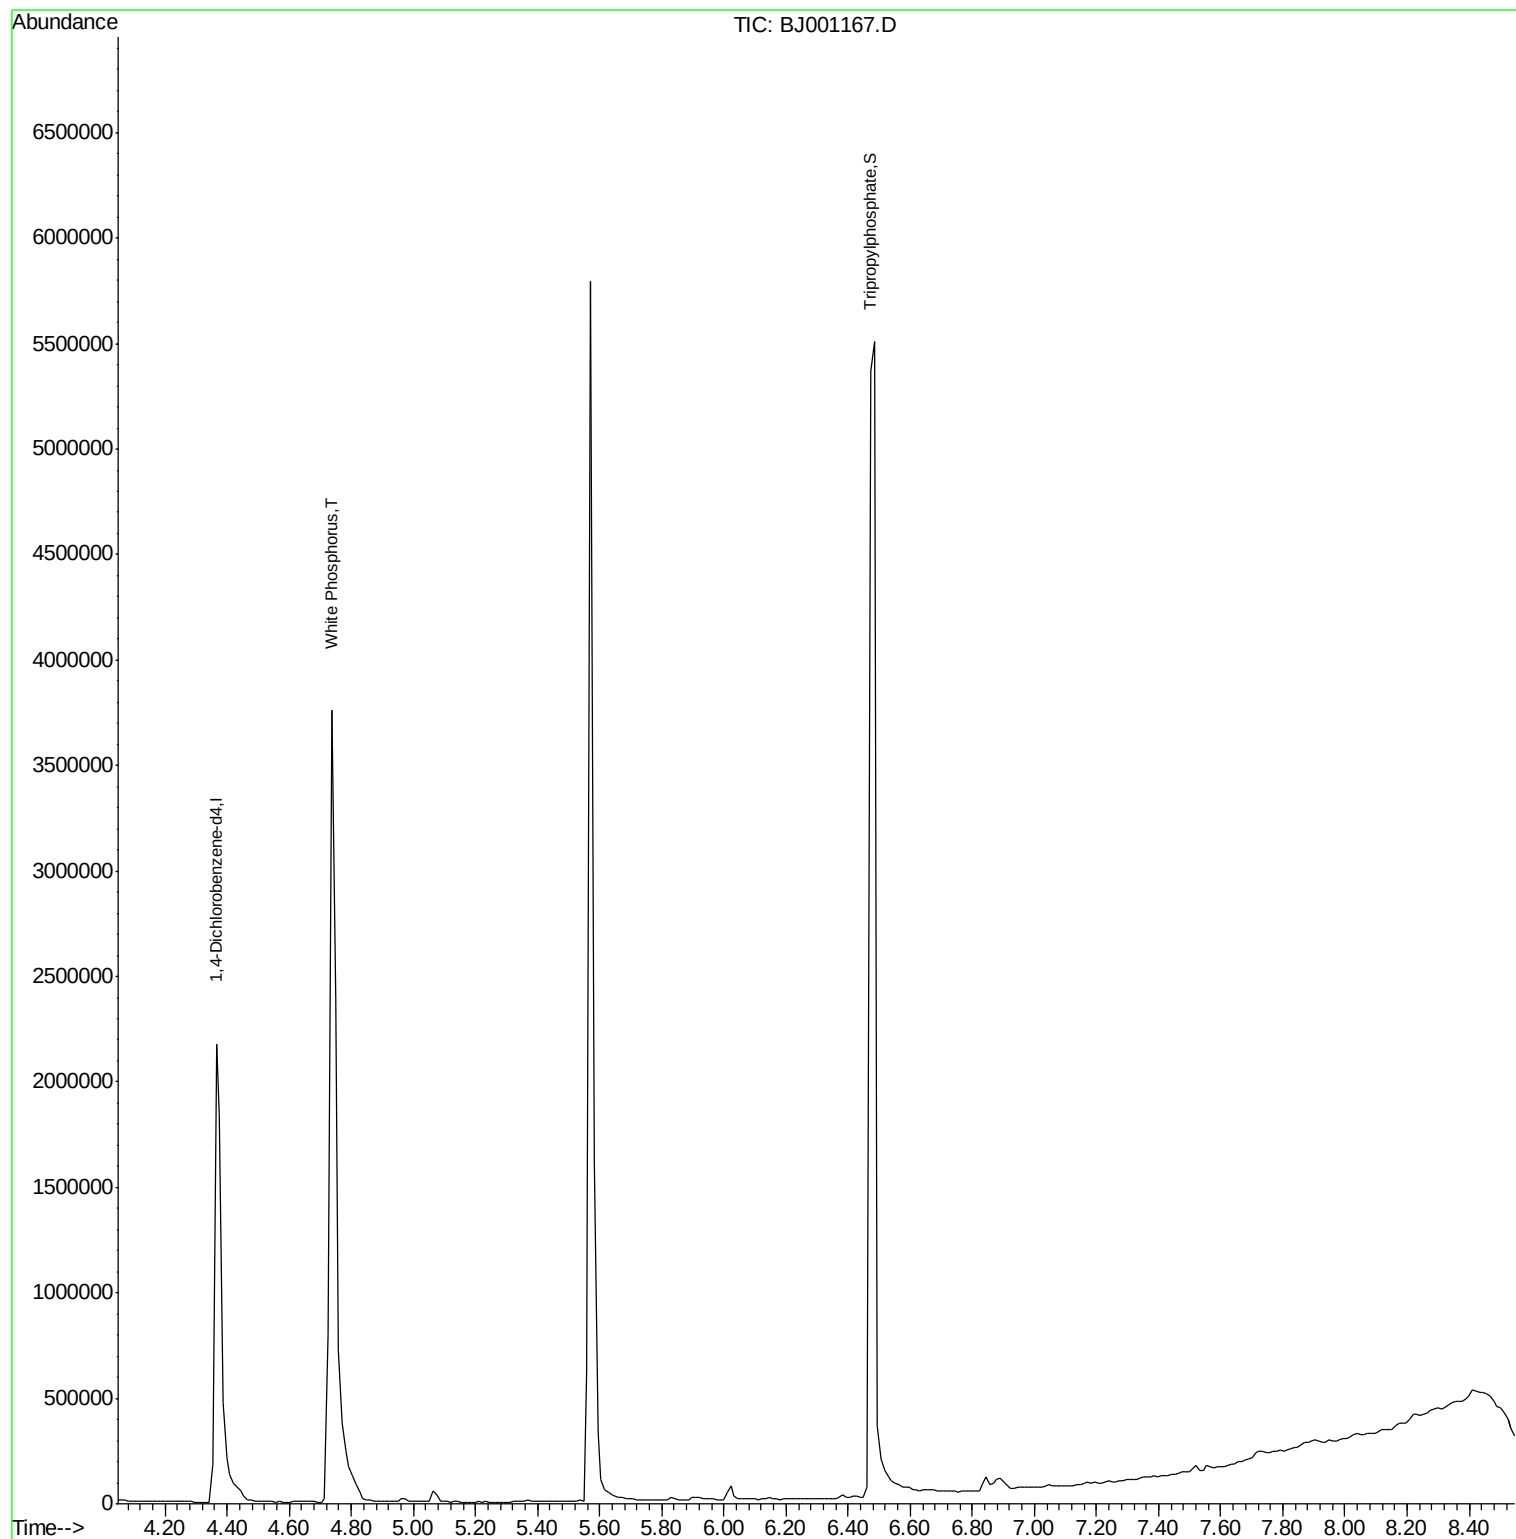


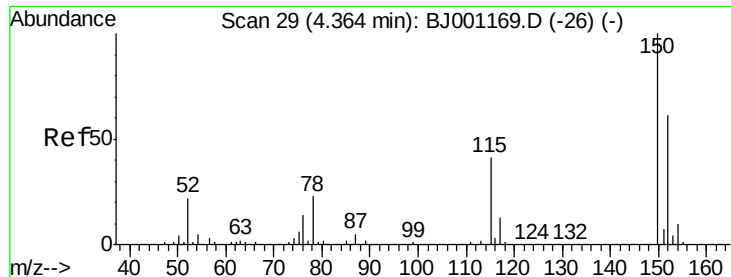




#1
 1,4-Dichlorobenzene-d4
 Concen: 2.50 ug/ml
 RT: 4.36 min Scan# 29
 Delta R.T. 0.00 min
 Lab File: BJ001167.D
 Acq: 4 Oct 2012 15:07

Instrument :
 BNA_J
 LabSampleId :
 P4-6

Tgt Ion:150 Resp: 1041933
 Ion Ratio Lower Upper
 150 100
 152 62.8 42.4 82.4

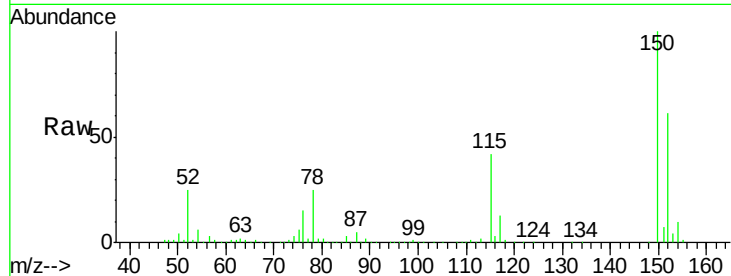


Abundance Ion 150.00 (149.70 to 150.70): E
 Ion 152.00 (151.70 to 152.70): E

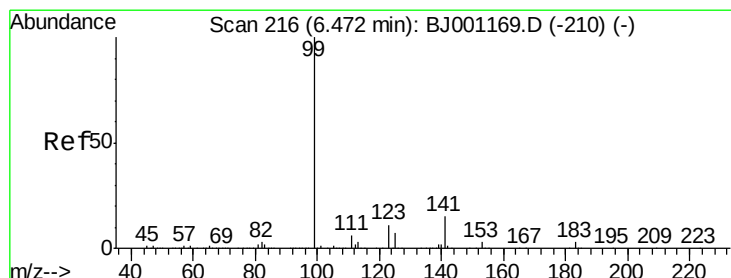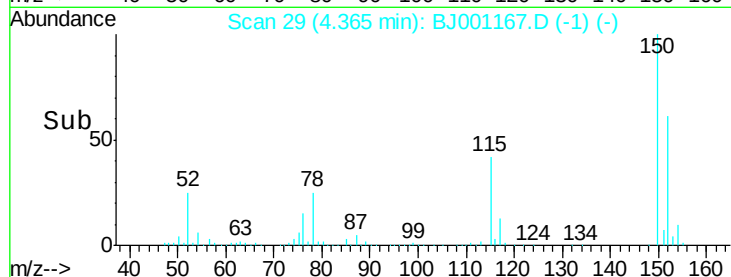
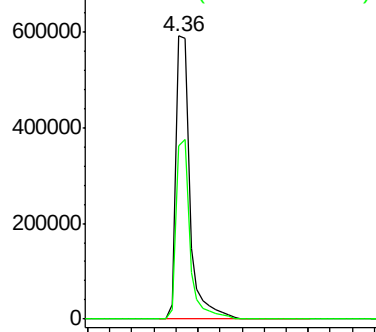



#2
 Tripropylphosphate
 Concen: 5.11 ug/ml
 RT: 6.47 min Scan# 216
 Delta R.T. 0.00 min
 Lab File: BJ001167.D
 Acq: 4 Oct 2012 15:07

Tgt Ion: 99 Resp: 4269718
 Ion Ratio Lower Upper
 99 100
 141 21.5 0.0 39.9

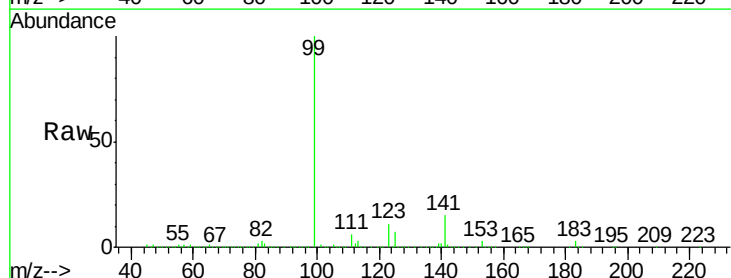

Abundance Ion 99.00 (98.70 to 99.70): BJ0
 Ion 141.00 (140.70 to 141.70): E

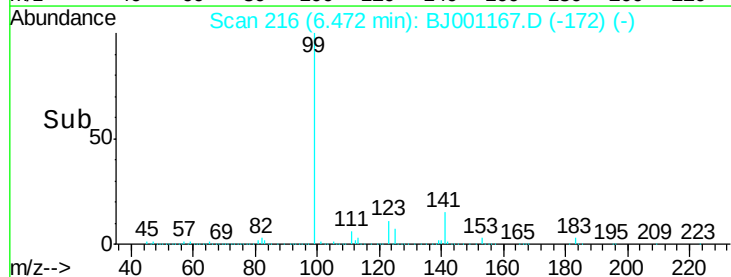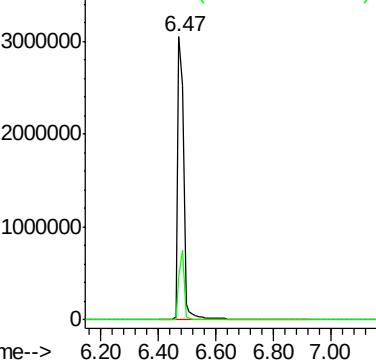


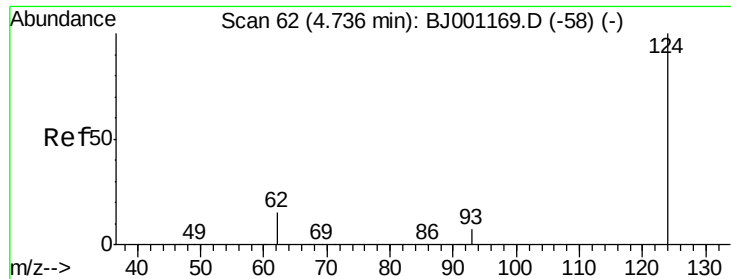

#3
 White Phosphorus
 Concen: 5.39 ug/ml
 RT: 4.74 min Scan# 62
 Delta R.T. 0.00 min
 Lab File: BJ001167.D
 Acq: 4 Oct 2012 15:07

Instrument :
 BNA_J
 LabSampleId :
 P4-6

Tgt Ion:124 Resp: 4852999
 Ion Ratio Lower Upper
 124 100
 93 7.1 0.0 27.3
 62 15.3 0.0 35.7

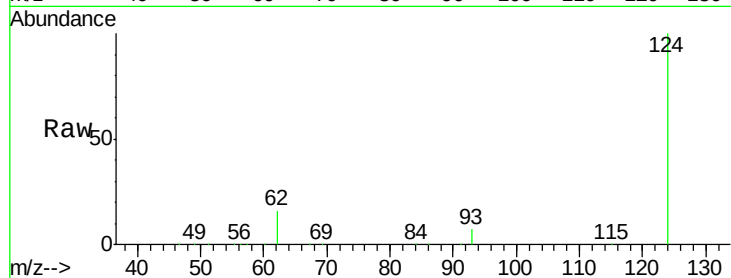

Abundance Ion 124.00 (123.70 to 124.70): E
 Ion 93.00 (92.70 to 93.70): BJ0
 Ion 62.00 (61.70 to 62.70): BJ0

