

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001169.D
Acq On : 4 Oct 2012 15:34
Operator : HLM
Sample : P4-4
Misc : BNA_J HLM
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-4

Quant Time: Oct 06 08:21:45 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	150	1302591	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	6.47	99	1137364	1.09	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	43.60%


Target Compounds					Qvalue
3) White Phosphorus	4.74	124	1259414	1.12	ug/ml 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001169.D
Acq On : 4 Oct 2012 15:34
Operator : HLM
Sample : P4-4
Misc : BNA_J HLM
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-4

Quant Time: Oct 06 08:21:45 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration

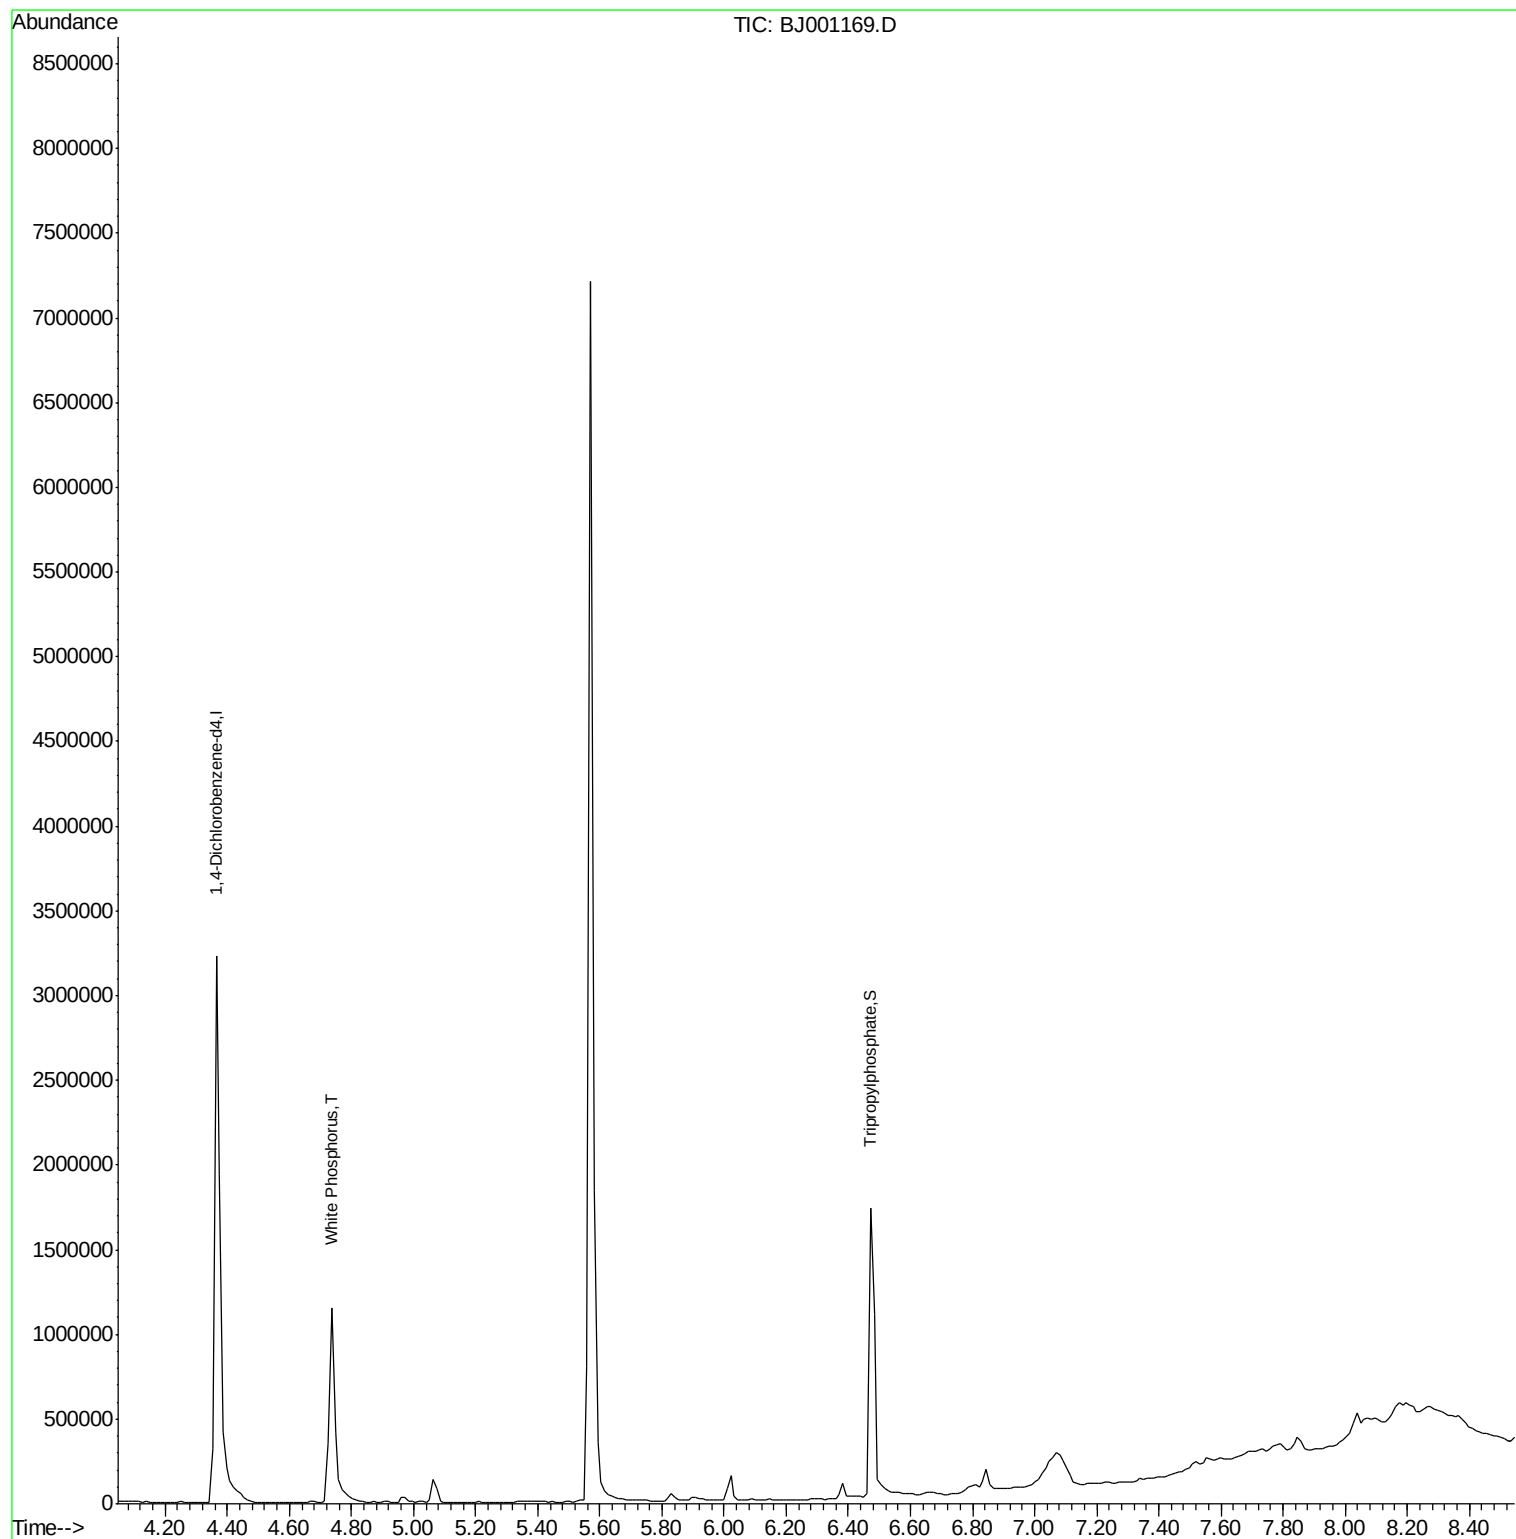

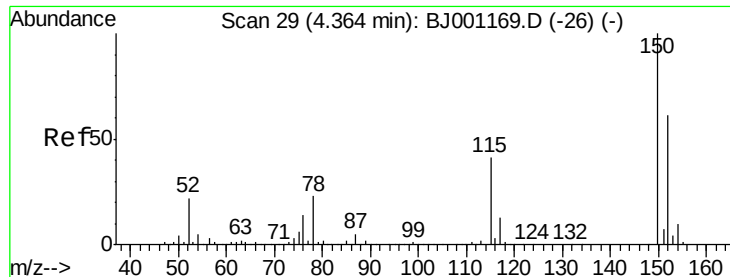


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.36 min Scan# 29
Delta R.T. 0.00 min
Lab File: BJ001169.D
Acq: 4 Oct 2012 15:34

Instrument :
BNA_J
LabSampleId :
P4-4

Tgt Ion:150 Resp: 1302591
Ion Ratio Lower Upper
150 100
152 62.4 42.4 82.4

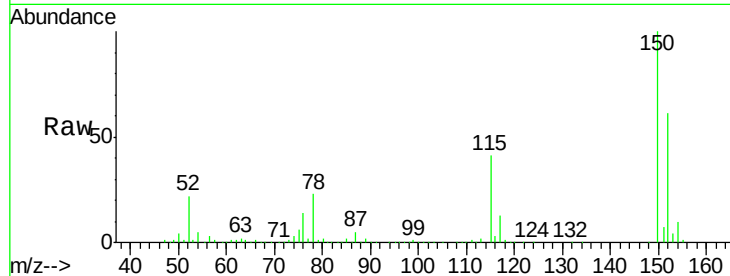


Abundance Ion 150.00 (149.70 to 150.70): B
Ion 152.00 (151.70 to 152.70): B

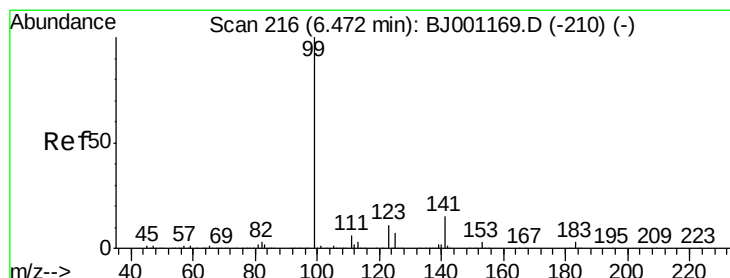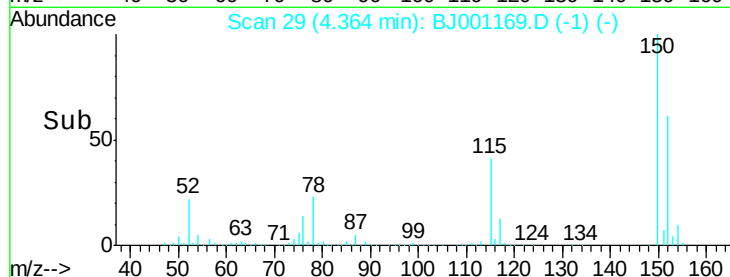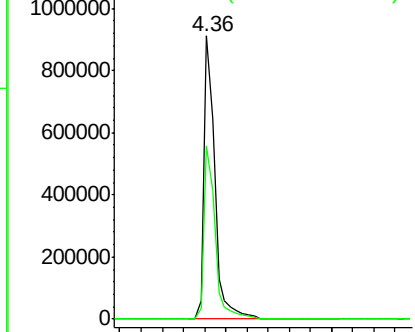



#2


Tripropylphosphate
Concen: 1.09 ug/ml
RT: 6.47 min Scan# 216
Delta R.T. 0.00 min
Lab File: BJ001169.D
Acq: 4 Oct 2012 15:34

Tgt Ion: 99 Resp: 1137364
Ion Ratio Lower Upper
99 100
141 19.9 0.0 39.9

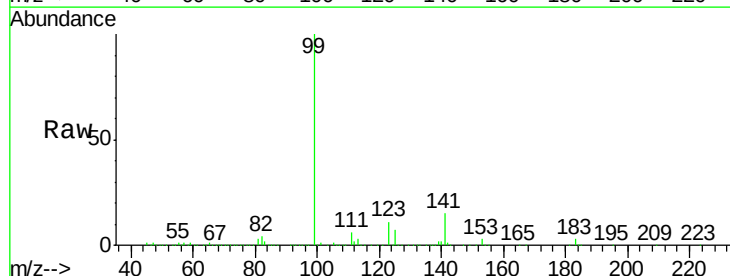

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): B

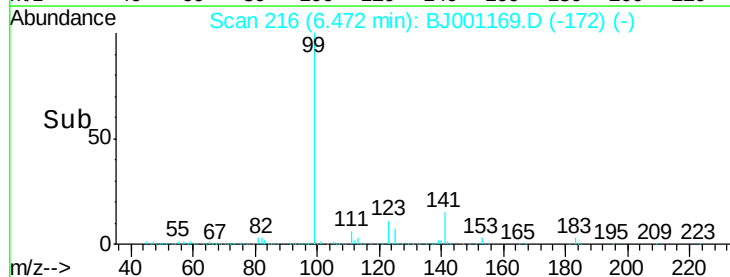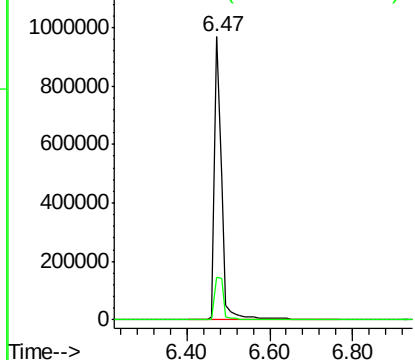


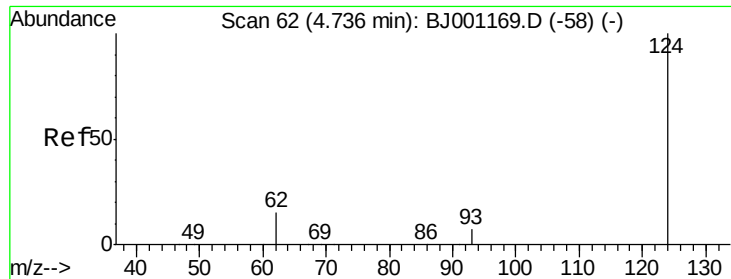

#3
 White Phosphorus
 Concen: 1.12 ug/ml
 RT: 4.74 min Scan# 62
 Delta R.T. 0.00 min
 Lab File: BJ001169.D
 Acq: 4 Oct 2012 15:34

Instrument :
 BNA_J
 LabSampleId :
 P4-4

Tgt Ion:124 Resp: 1259414
 Ion Ratio Lower Upper
 124 100
 93 7.3 0.0 27.3
 62 15.7 0.0 35.7

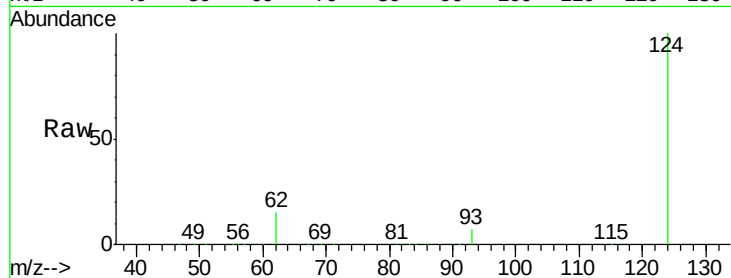

Abundance Ion 124.00 (123.70 to 124.70): E
 Ion 93.00 (92.70 to 93.70): BJ0
 Ion 62.00 (61.70 to 62.70): BJ0

