

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001170.D
Acq On : 4 Oct 2012 15:46
Operator : HLM
Sample : P4-3
Misc : BNA_J HLM
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-3

Quant Time: Oct 06 08:25:04 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	150	1181822	2.50	ug/ml	0.00

System Monitoring Compounds
2) Tripropylphosphate 6.47 99 533163 0.56 ug/ml 0.00
Spiked Amount 2.500 Range 20 - 150 Recovery = 22.40%


Target Compounds					Qvalue
3) White Phosphorus	4.74	124	559960	0.55 ug/ml	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001170.D
Acq On : 4 Oct 2012 15:46
Operator : HLM
Sample : P4-3
Misc : BNA_J HLM
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-3

Quant Time: Oct 06 08:25:04 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:38:53 2012
Response via : Initial Calibration

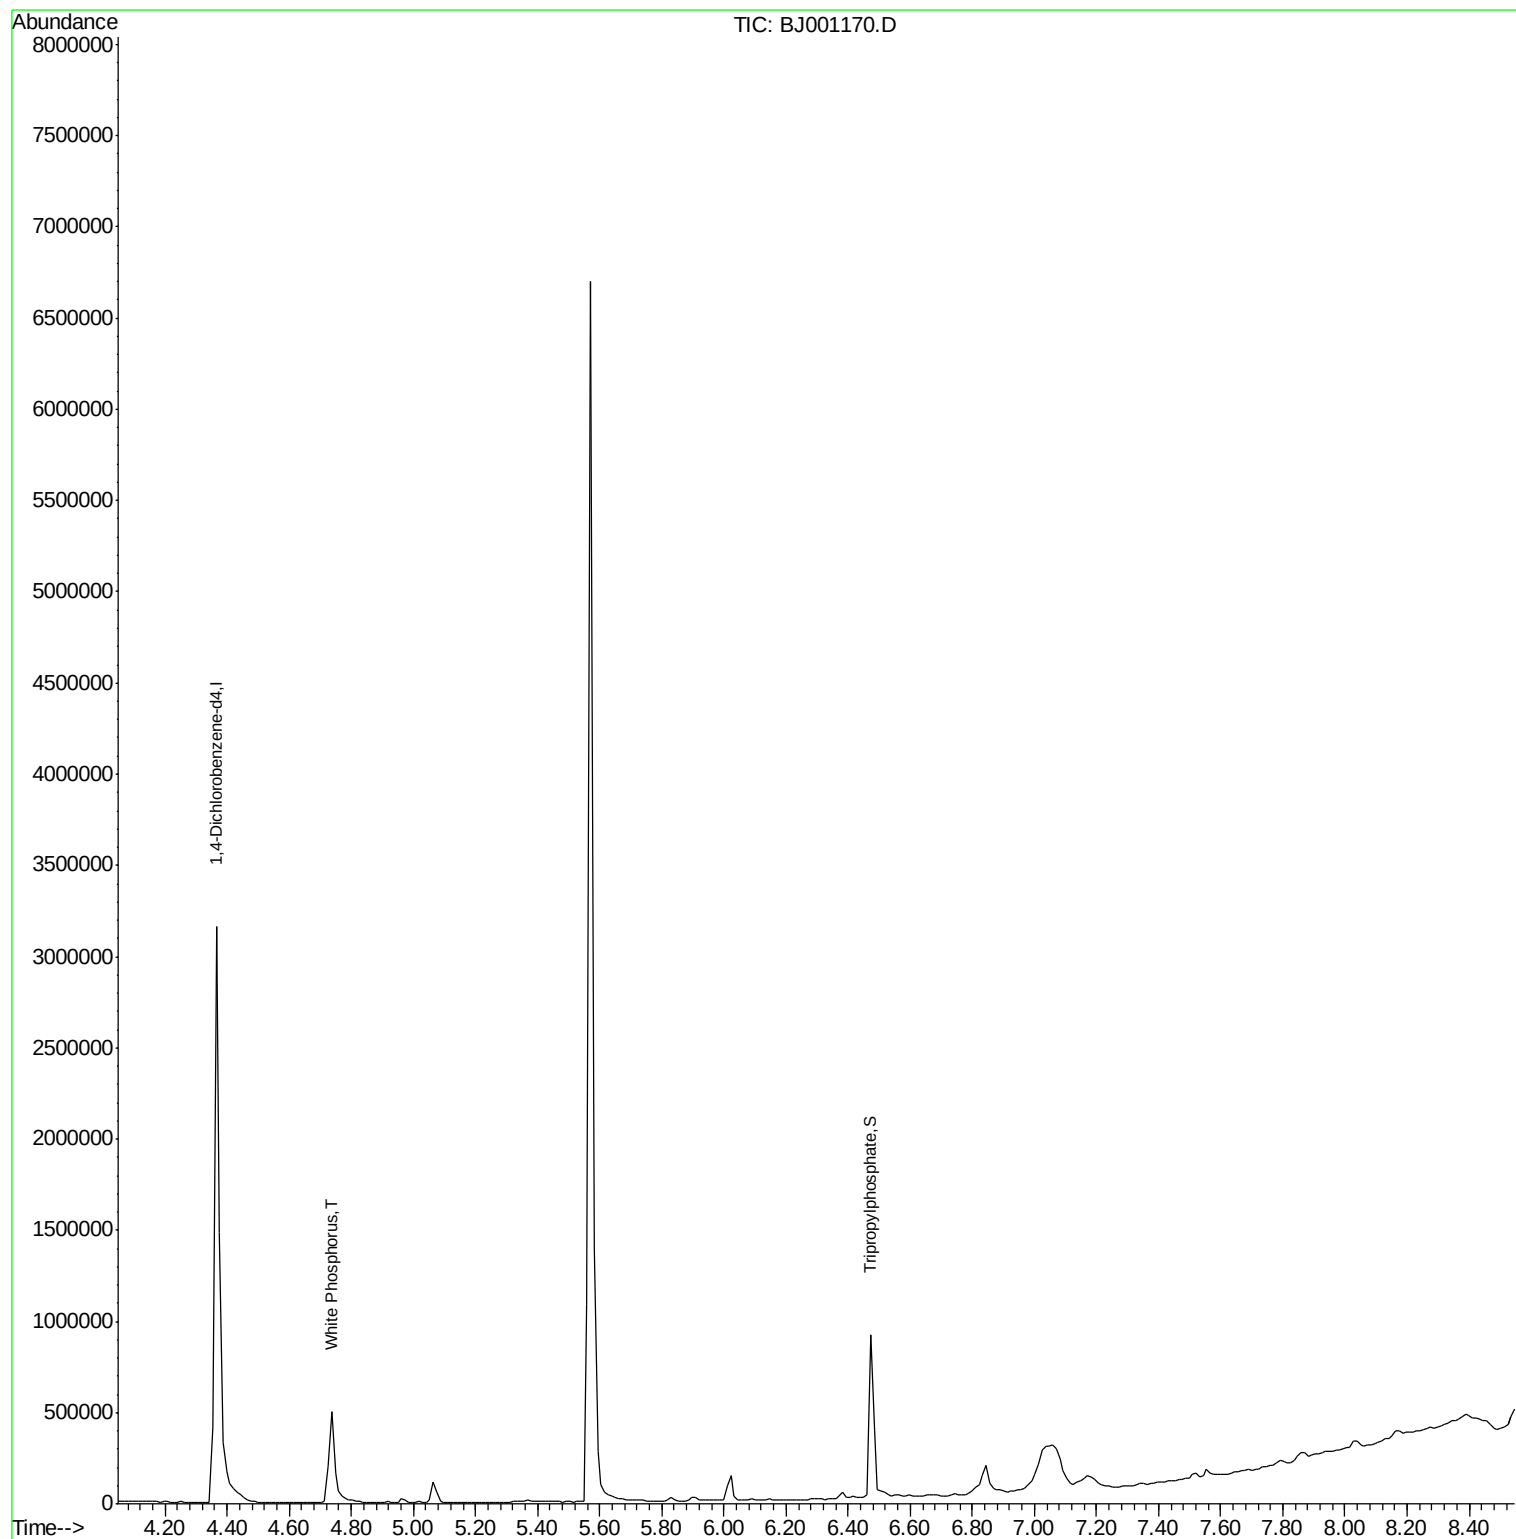

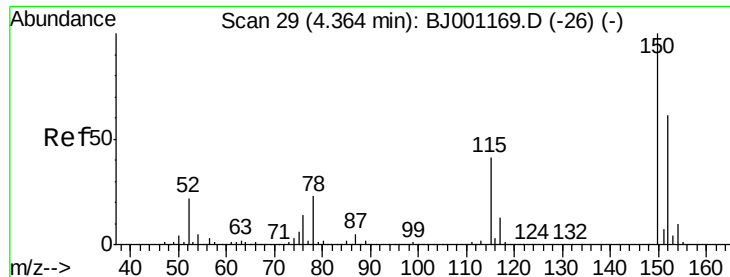


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.36 min Scan# 29
Delta R.T. 0.00 min
Lab File: BJ001170.D
Acq: 4 Oct 2012 15:46

Instrument :
BNA_J
LabSampleId :
P4-3

Tgt Ion:150 Resp: 1181822
Ion Ratio Lower Upper
150 100
152 62.6 42.4 82.4

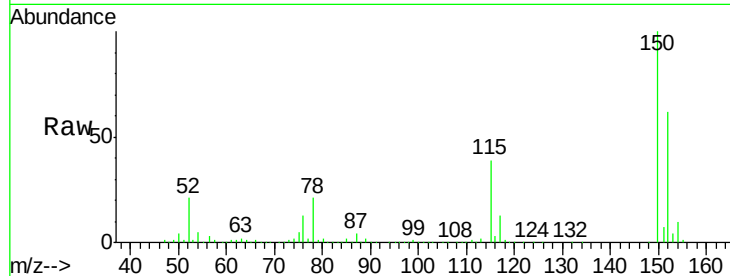


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

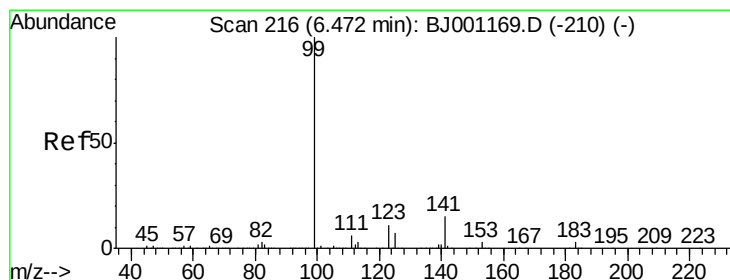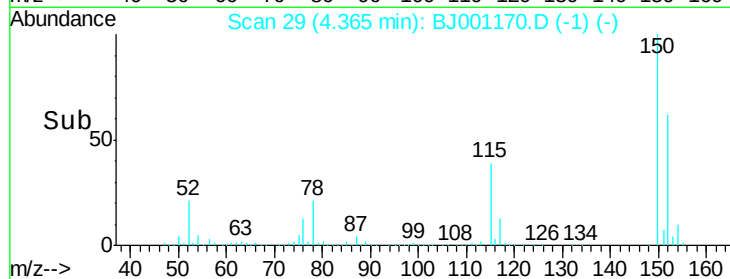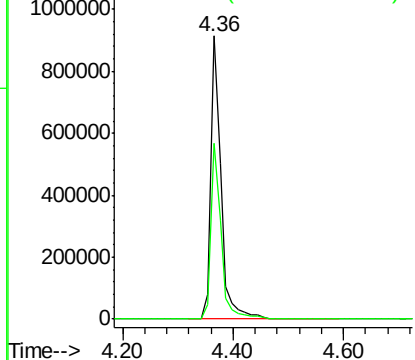



#2


Tripropylphosphate
Concen: 0.56 ug/ml
RT: 6.47 min Scan# 216
Delta R.T. 0.00 min
Lab File: BJ001170.D
Acq: 4 Oct 2012 15:46

Tgt Ion: 99 Resp: 533163
Ion Ratio Lower Upper
99 100
141 19.6 0.0 39.9

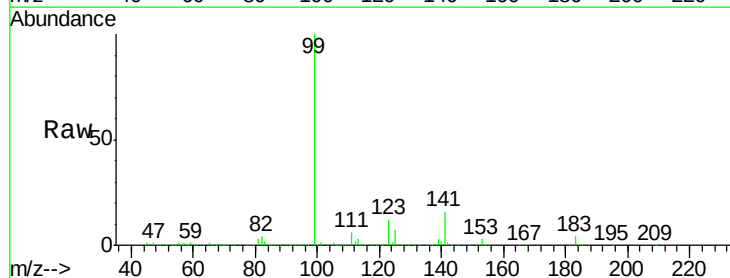

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

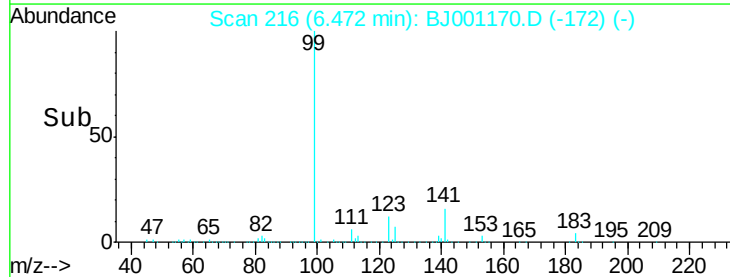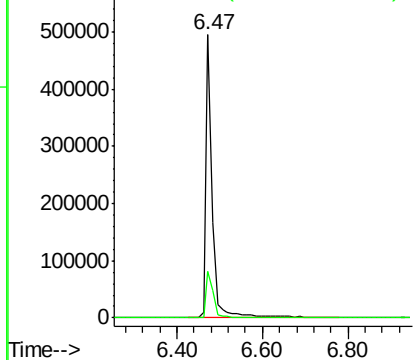

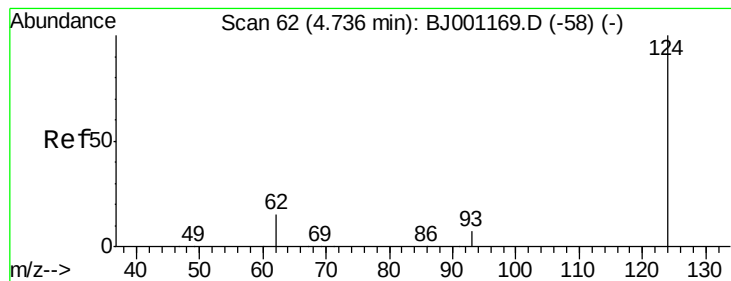

#3

White Phosphorus

Concen: 0.55 ug/ml

RT: 4.74 min Scan# 62

Delta R.T. 0.00 min

Lab File: BJ001170.D


Acq: 4 Oct 2012 15:46

Instrument :

BNA_J

LabSampleId :

P4-3

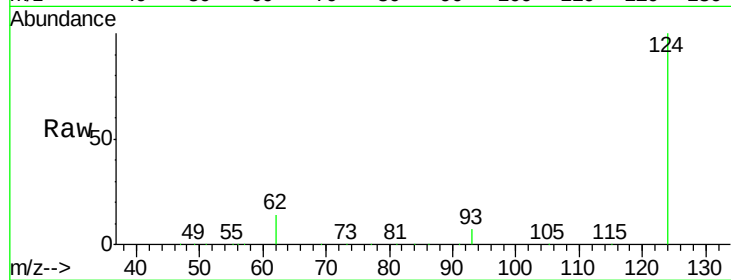


Tgt Ion:124 Resp: 559960

Ion Ratio Lower Upper

124 100

93 7.4 0.0 27.3

62 15.6 0.0 35.7

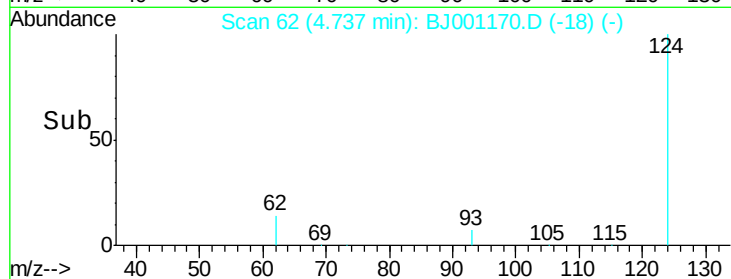

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

