

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001173.D
Acq On : 4 Oct 2012 16:26
Operator : HLM
Sample : P4-ICV
Misc : BNA_J HLM
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-ICV

Quant Time: Oct 06 08:25:10 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:45:25 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	150	973970	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	0.00	99	0	0.00	ug/ml	
Spiked Amount	2.500	Range	20 - 150	Recovery	=	0.00%#

Target Compounds


3) White Phosphorus	4.74	124	861130	0.94	ug/ml	Qvalue 99
---------------------	------	-----	--------	------	-------	-----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001173.D
Acq On : 4 Oct 2012 16:26
Operator : HLM
Sample : P4-ICV
Misc : BNA_J HLM
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-ICV

Quant Time: Oct 06 08:25:10 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:45:25 2012
Response via : Initial Calibration

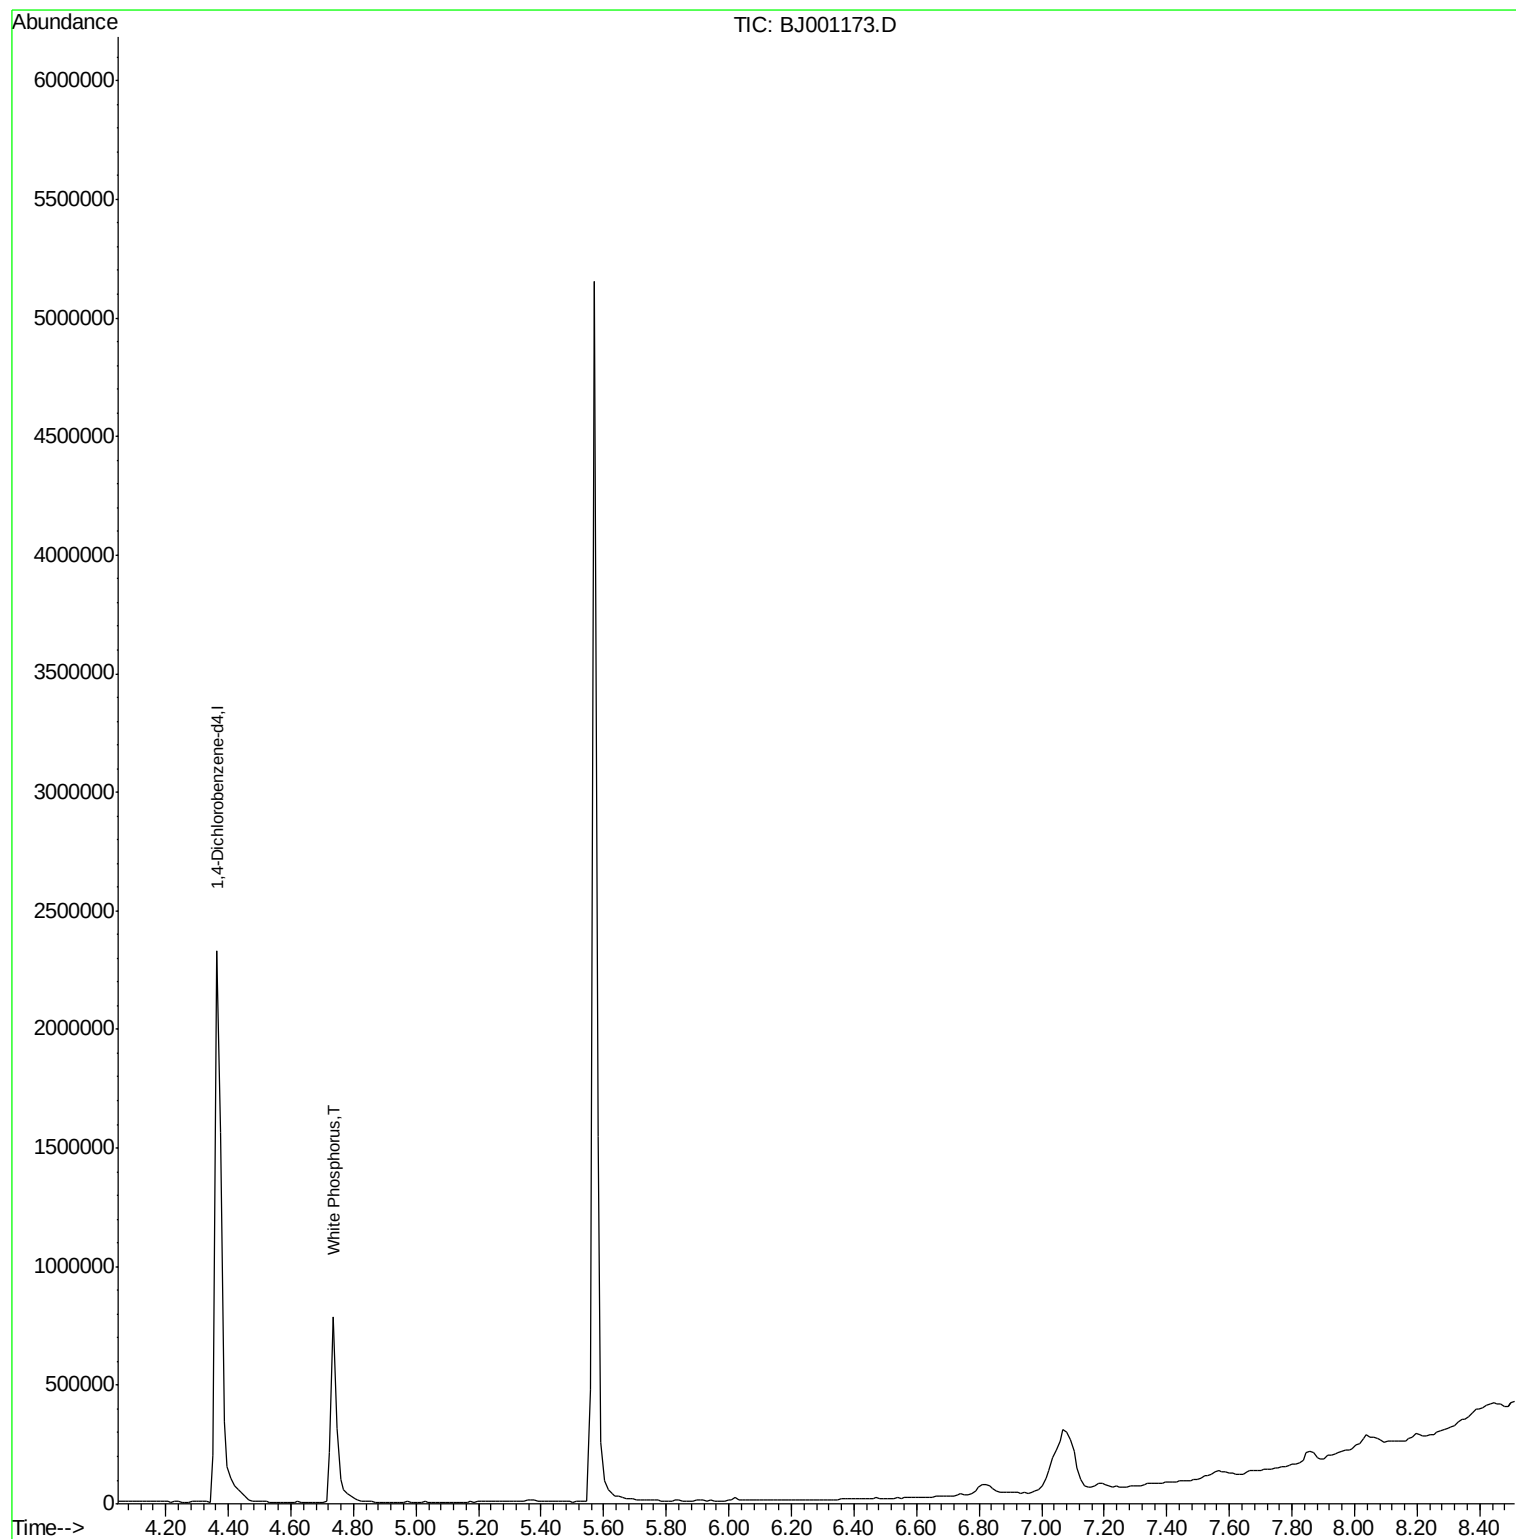

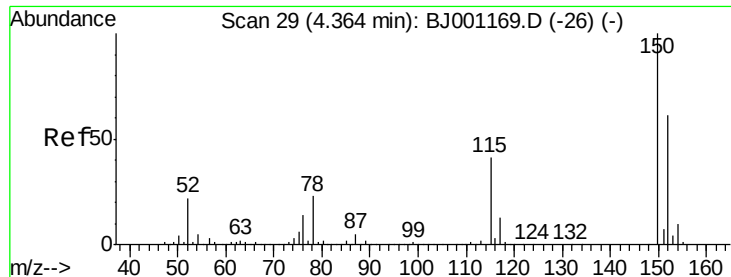


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.36 min Scan# 29
Delta R.T. -0.00 min
Lab File: BJ001173.D
Acq: 4 Oct 2012 16:26

Instrument :
BNA_J
ClientSampleId :
P4-ICV

Tgt Ion:150 Resp: 973970
Ion Ratio Lower Upper
150 100
152 62.5 42.4 82.4

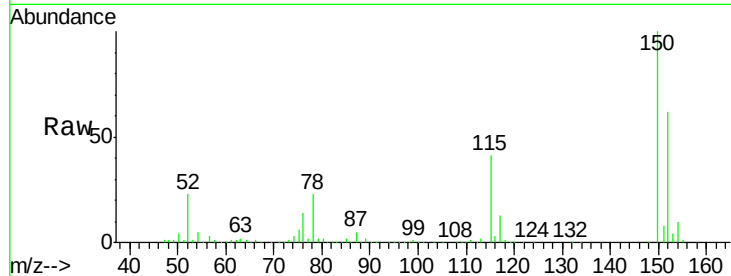

Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

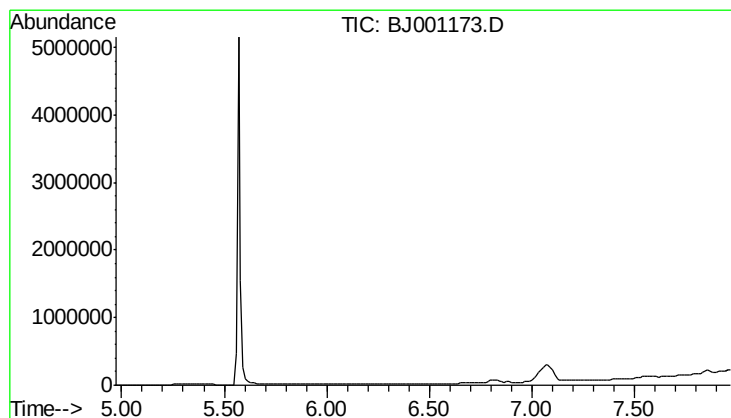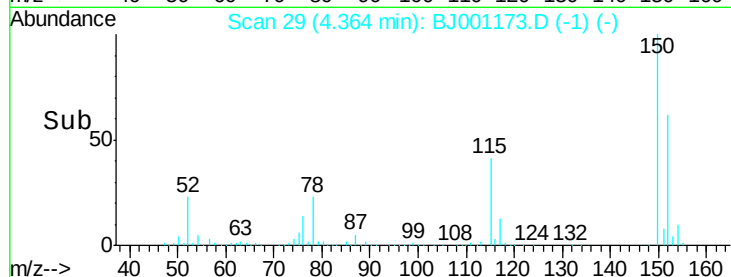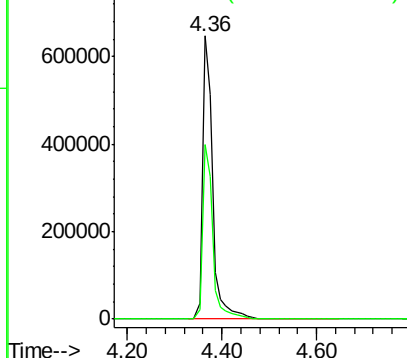



#2

Tripropylphosphate
Concen: 0.00 ug/ml
Expected RT: 6.47 min

Lab File: BJ001173.D
Acq: 4 Oct 2012 16:26

Tgt Ion: 99
Sig Exp Ratio
99 100
141 19.9

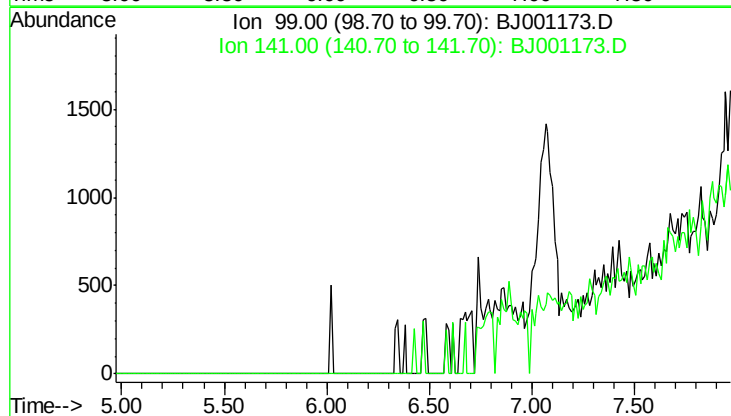

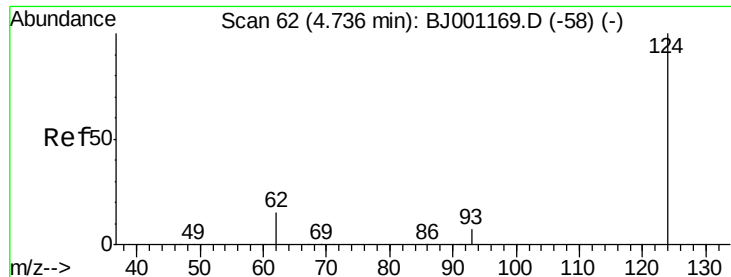

#3
 White Phosphorus
 Concen: 0.94 ug/ml
 RT: 4.74 min Scan# 62
 Delta R.T. -0.00 min
 Lab File: BJ001173.D
 Acq: 4 Oct 2012 16:26

Instrument :
 BNA_J
 ClientSampleId :
 P4-ICV

Tgt Ion:	124	Resp:	861130
Ion	Ratio	Lower	Upper
124	100		
93	7.2	0.0	27.3
62	15.3	0.0	35.7

