

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001179.D
Acq On : 4 Oct 2012 19:40
Operator : HLM
Sample : D4310-02
Misc : SOIL BNA_J HLM
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
LG523-02-SS01-B

Manual Integrations

APPROVED
AHPatel
10/9/2012 7:06:44 AM

Quant Time: Oct 06 08:25:46 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:46:22 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.37	150	986021	2.50	ug/ml	0.01

System Monitoring Compounds

2) Tripropylphosphate	6.49	99	1542618	1.85	ug/ml	0.02
Spiked Amount	2.500	Range	20 - 150	Recovery	=	74.00%

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001179.D
Acq On : 4 Oct 2012 19:40
Operator : HLM
Sample : D4310-02
Misc : SOIL BNA_J HLM
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_J
ClientSampleId :
LG523-02-SS01-B

Manual Integrations

APPROVED
AHPatel
10/9/2012 7:06:44 AM

Quant Time: Oct 06 08:25:46 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:46:22 2012
Response via : Initial Calibration

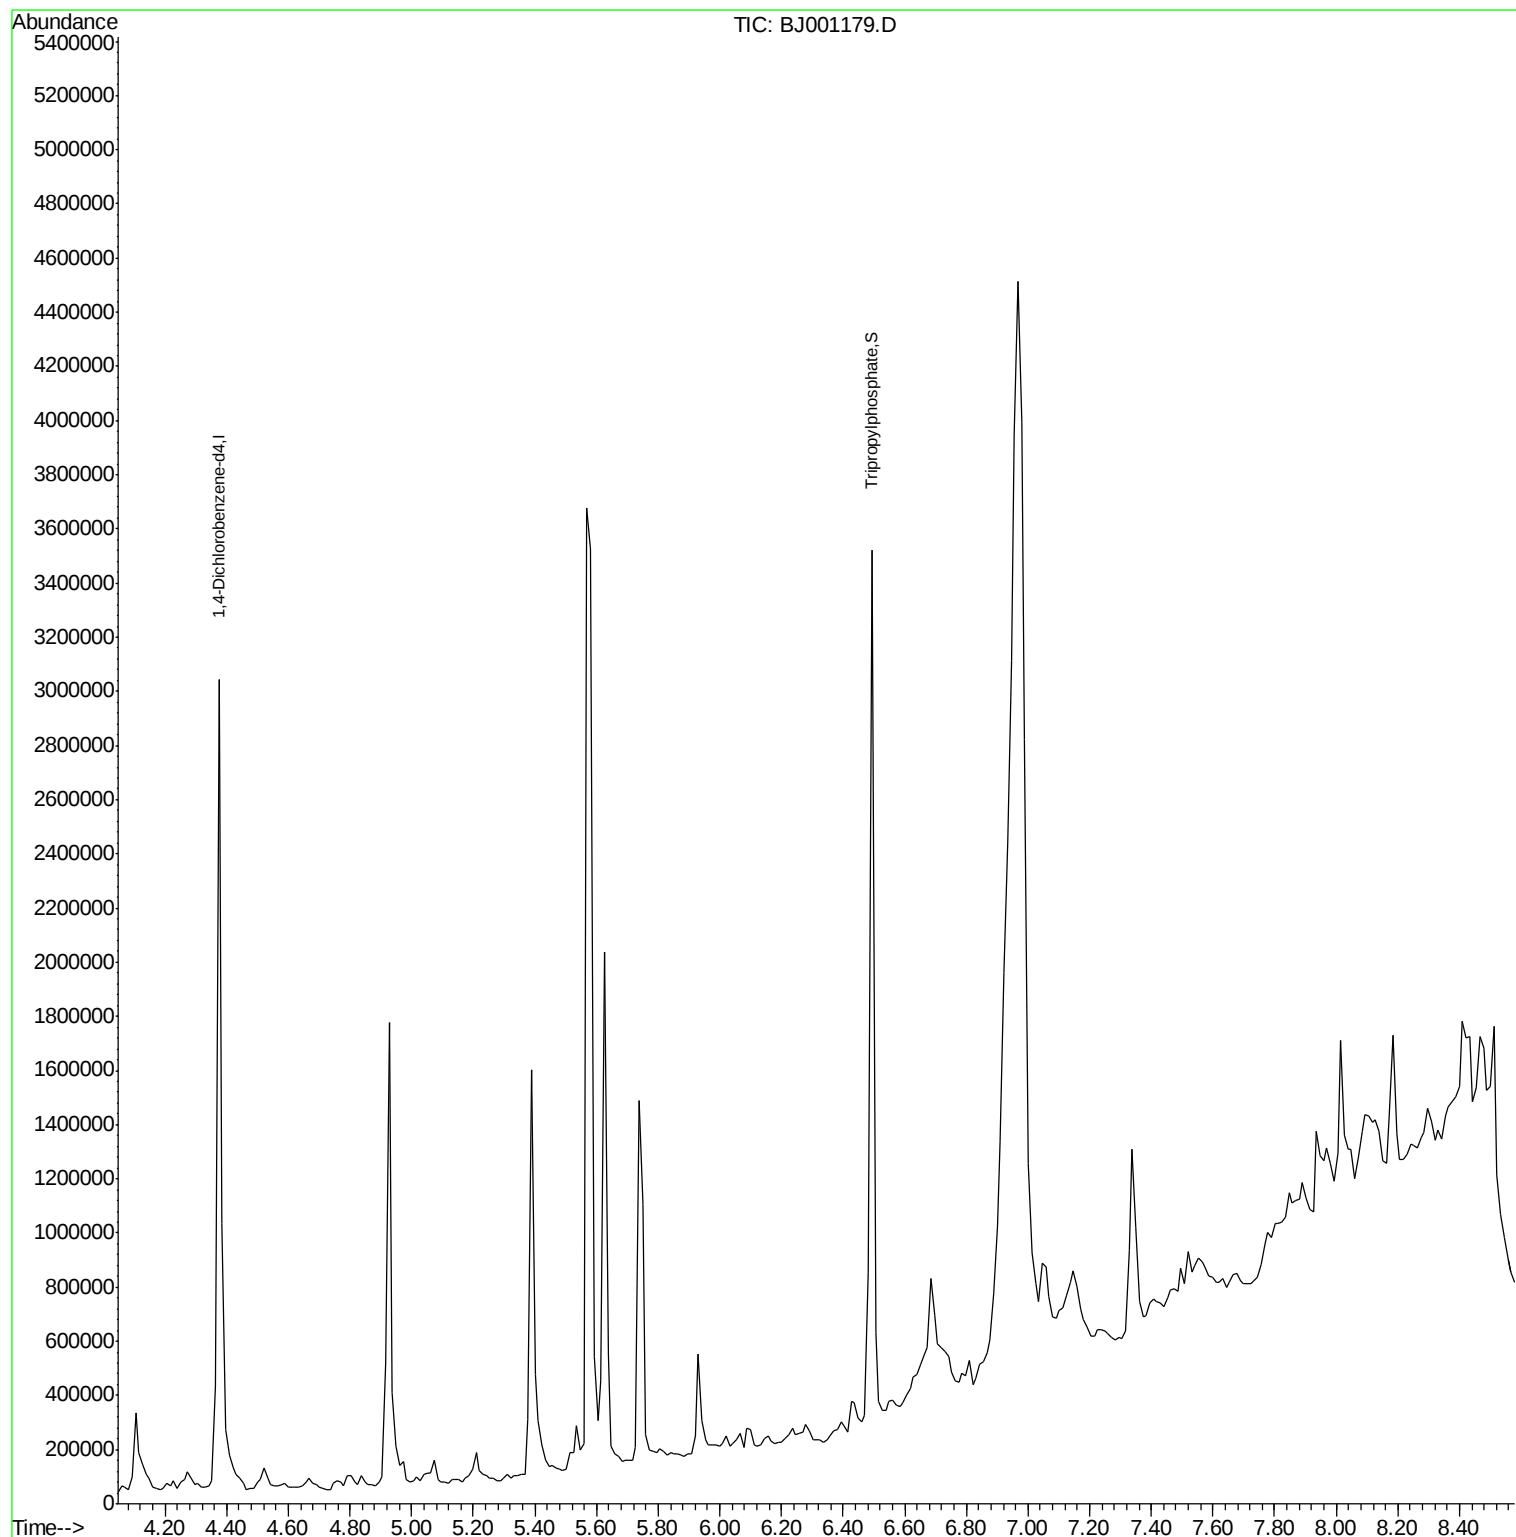

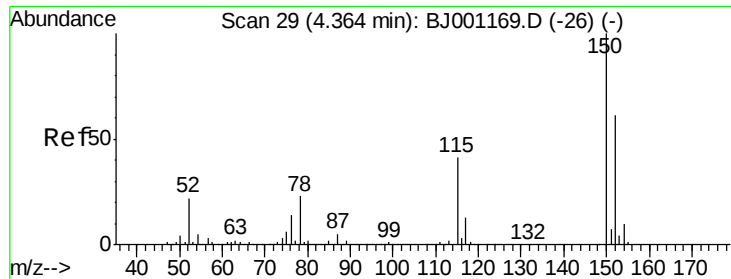

#1





1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.37 min Scan# 30
Delta R.T. 0.01 min
Lab File: BJ001179.D
Acq: 4 Oct 2012 19:40

Instrument :
BNA_J
ClientSampleId :
LG523-02-SS01-B

Tgt Ion:150 Resp: 986021
Ion Ratio Lower Upper
150 100
152 63.0 42.4 82.4

Manual Integrations

APPROVED
AHPatel
10/9/2012 7:06:44 AM

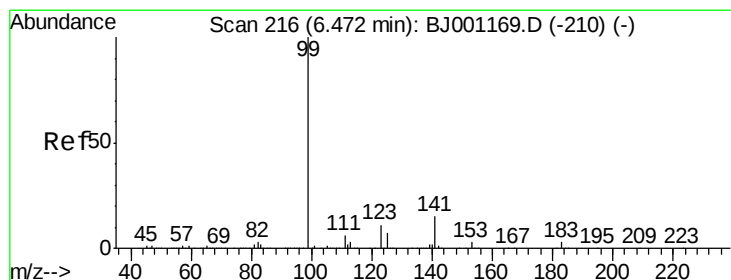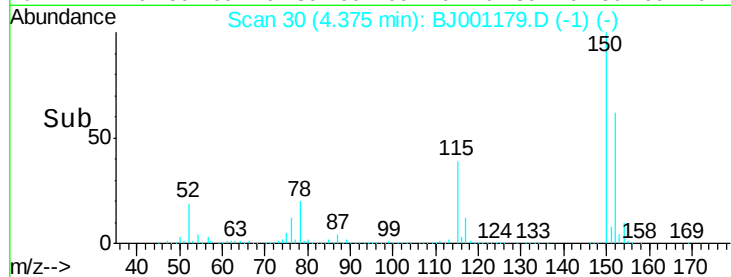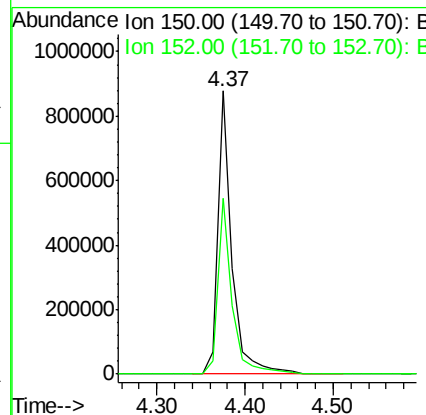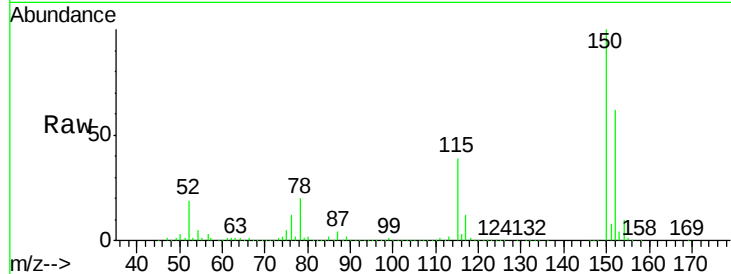

#2

Tripropylphosphate
Concen: 1.85 ug/ml
RT: 6.49 min Scan# 218
Delta R.T. 0.02 min
Lab File: BJ001179.D
Acq: 4 Oct 2012 19:40

Tgt Ion: 99 Resp: 1542618
Ion Ratio Lower Upper
99 100
141 20.7 0.0 39.9

