

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001183.D
Acq On : 4 Oct 2012 20:32
Operator : HLM
Sample : PB66027BS
Misc : SOIL BNA_J HLM
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
SLCS02

Quant Time: Oct 06 08:25:54 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:46:22 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.37	150	960444	2.50	ug/ml	0.01

System Monitoring Compounds

2) Tripropylphosphate	6.49	99	1746419	2.15	ug/ml	0.02
Spiked Amount	2.500	Range	20 - 150	Recovery	=	86.00%


Target Compounds					Qvalue
3) White Phosphorus	4.75	124	266334	0.29	ug/ml 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
Data File : BJ001183.D
Acq On : 4 Oct 2012 20:32
Operator : HLM
Sample : PB66027BS
Misc : SOIL BNA_J HLM
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
SLCS02

Quant Time: Oct 06 08:25:54 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ100412.M
Quant Title : P4 by SOP M.5
QLast Update : Thu Oct 04 17:46:22 2012
Response via : Initial Calibration

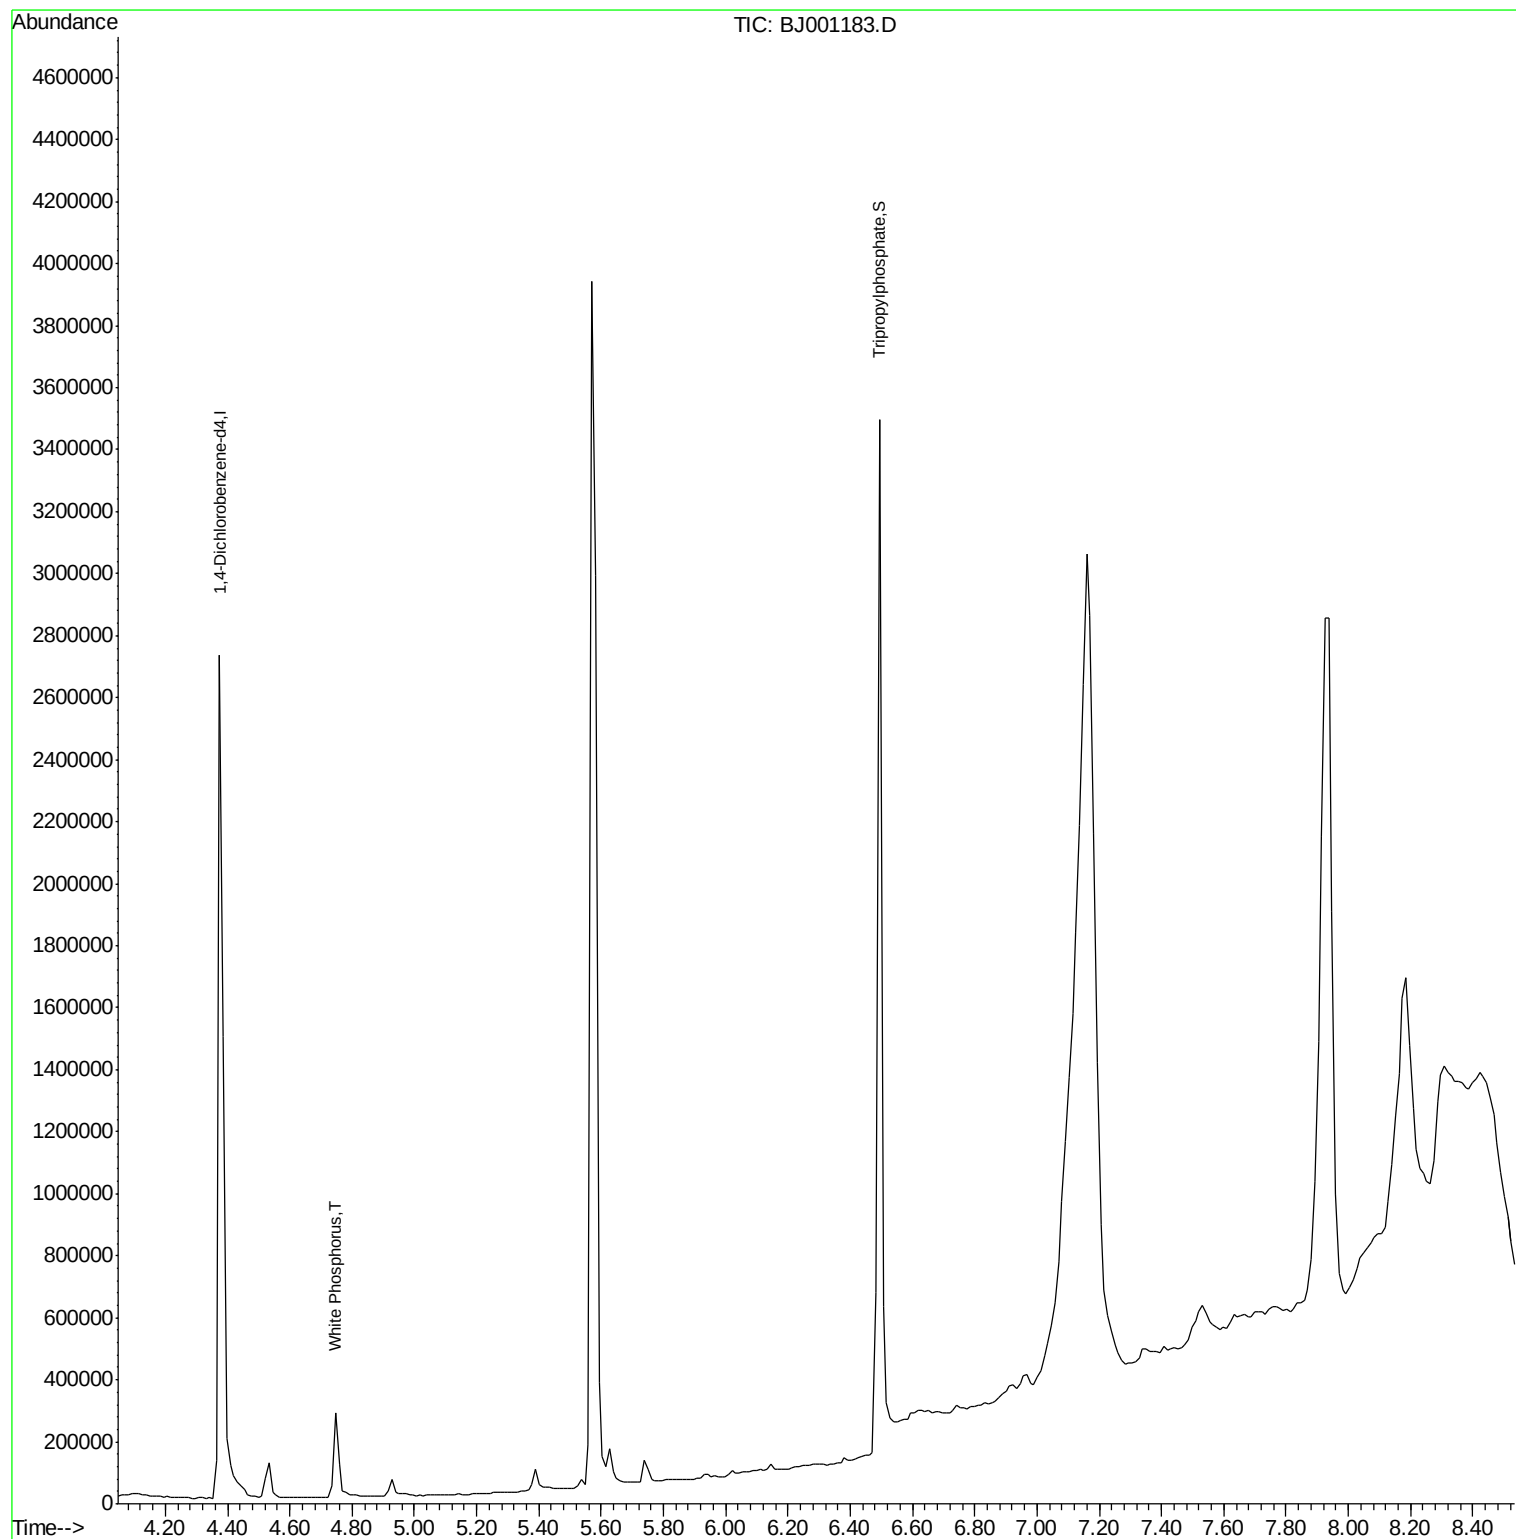

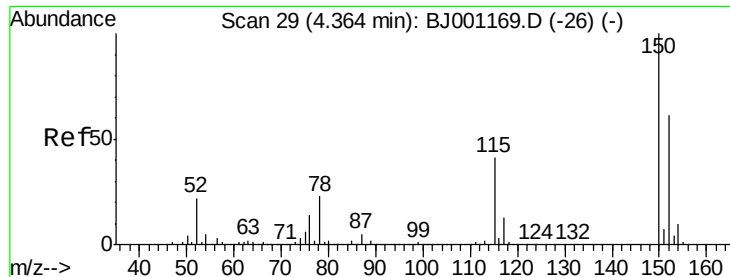


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.37 min Scan# 30
Delta R.T. 0.01 min
Lab File: BJ001183.D
Acq: 4 Oct 2012 20:32

Instrument :
BNA_J
ClientSampleId :
SLCS02

Tgt Ion:150 Resp: 960444
Ion Ratio Lower Upper
150 100
152 62.8 42.4 82.4

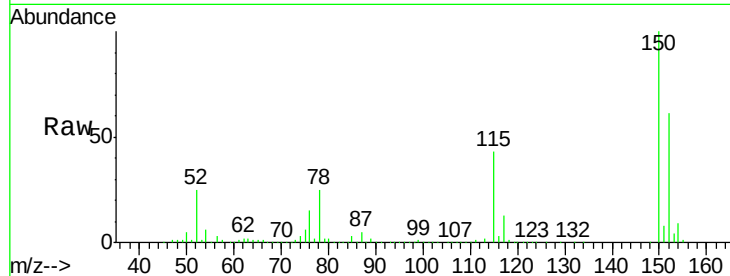


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

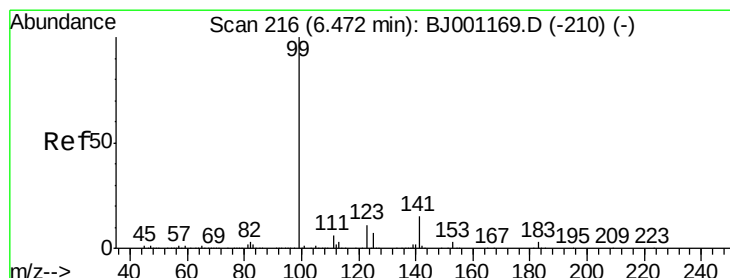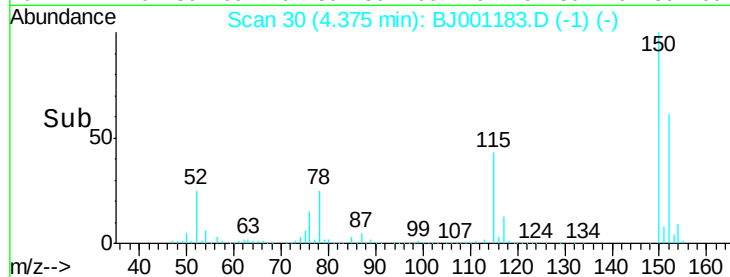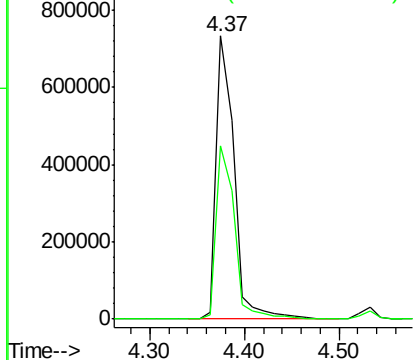



#2


Tripropylphosphate
Concen: 2.15 ug/ml
RT: 6.49 min Scan# 218
Delta R.T. 0.02 min
Lab File: BJ001183.D
Acq: 4 Oct 2012 20:32

Tgt Ion: 99 Resp: 1746419
Ion Ratio Lower Upper
99 100
141 21.2 0.0 39.9

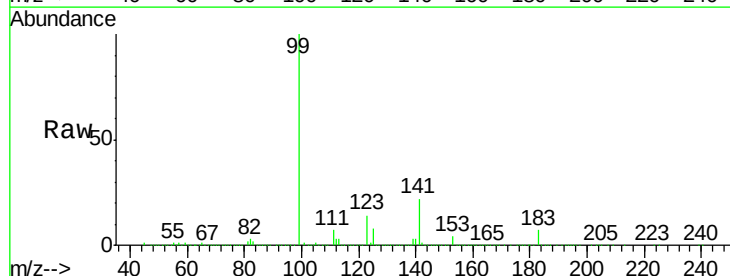

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

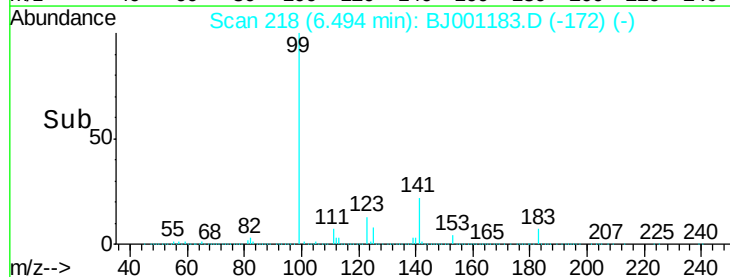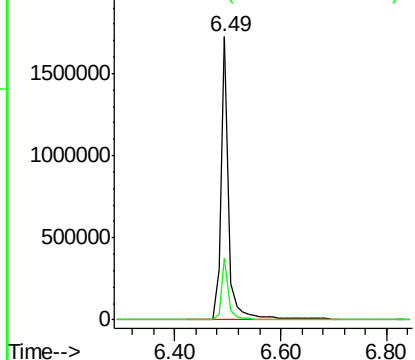

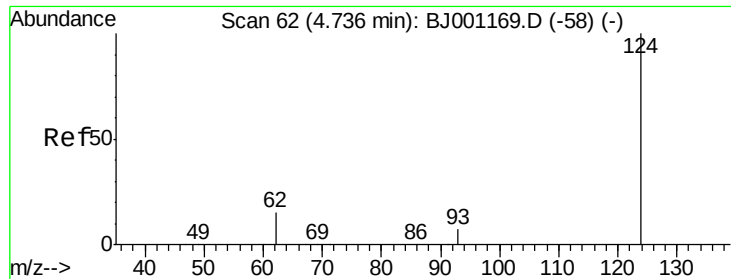

#3
 White Phosphorus
 Concen: 0.29 ug/ml
 RT: 4.75 min Scan# 63
 Delta R.T. 0.01 min
 Lab File: BJ001183.D
 Acq: 4 Oct 2012 20:32

Instrument :
 BNA_J
 ClientSampleId :
 SLCS02

Tgt Ion:	124	Resp:	266334
Ion	Ratio	Lower	Upper
124	100		
93	7.9	0.0	27.3
62	16.3	0.0	35.7

