


Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ100412\
 Data File : BJ001165.D
 Acq On : 4 Oct 2012 12:25
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_J\METHOD\BJ100412.M
 Title : P4 by SOP M.5
 Last Update : Thu Oct 04 17:45:25 2012

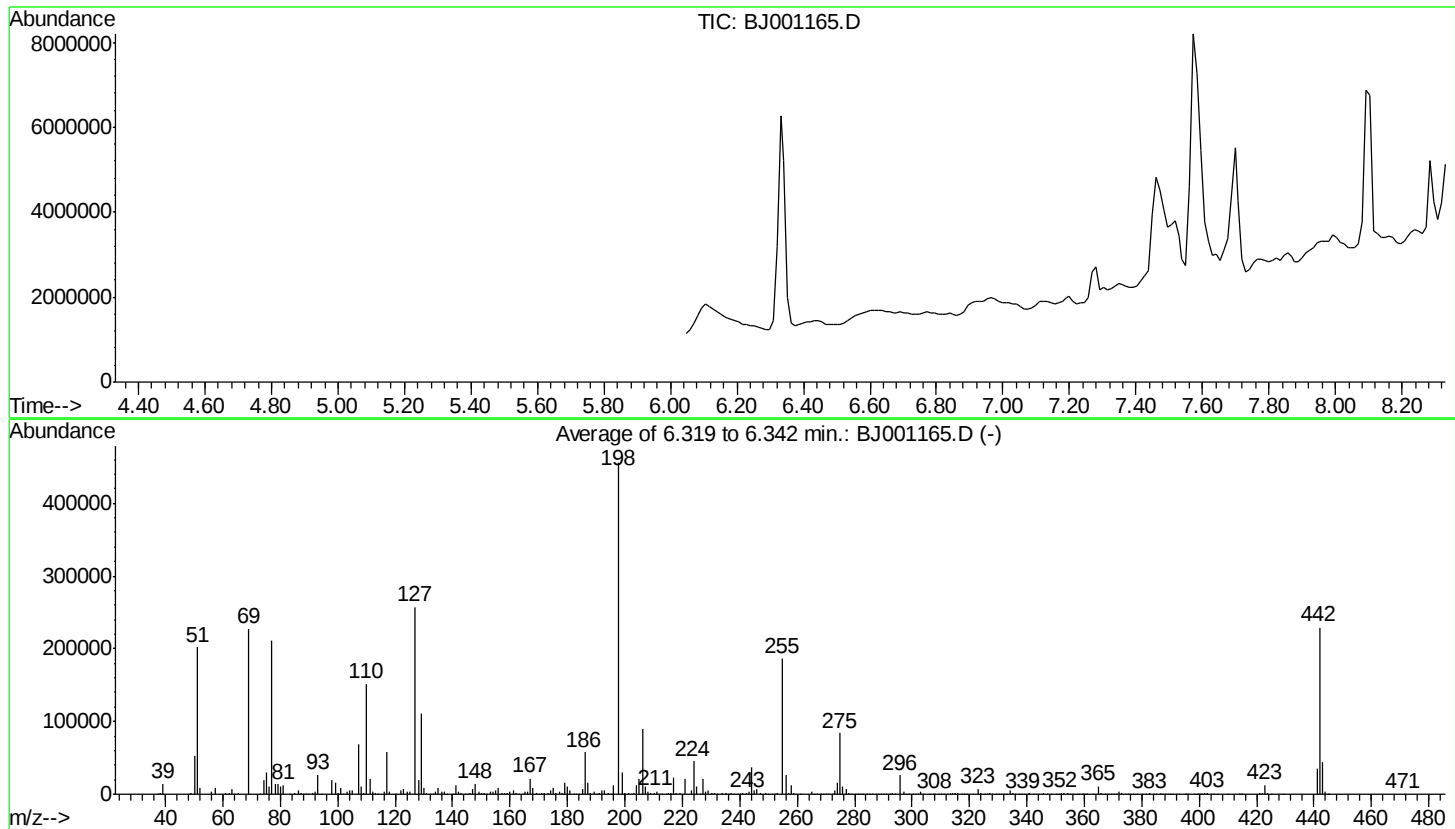

AutoFind: Scans 25, 26, 27; Background Corrected with Scan 21

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.2	201650	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.9	227360	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	56.5	257715	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	455818	PASS
199	198	5	9	6.5	29591	PASS
275	198	10	30	18.5	84385	PASS
365	198	1	100	2.4	10879	PASS
441	443	0.01	100	78.7	34596	PASS
442	198	40	100	50.2	229021	PASS
443	442	17	23	19.2	43940	PASS