

Data File : H:\VOL1\GCMSDATA\J\121112\BJ001203.D  
Acq On : 12 Nov 2012 15:29  
Sample : P4-1  
Misc : P4 BNA J HLM  
MS Integration Params: RTEINT.P  
Quant Time: Nov 12 15:55 2012

Vial: 32  
Operator: HLM  
Inst : BNA J  
Multiplr: 1.00

Instrument :  
BNA\_J  
LabSampleId :  
P4-1

Quant Results File: BJ111212.PRES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)  
Title : P4 by SOP M.5  
Last Update : Mon Nov 12 15:55:37 2012  
Response via : Initial Calibration  
DataAcq Meth : P4

| Internal Standards          | R.T.  | QIon  | Response | Conc     | Units | Dev(Min)      |
|-----------------------------|-------|-------|----------|----------|-------|---------------|
| 1) 1,4-Dichlorobenzene-d4   | 4.38  | 150   | 975710   | 2.50     | ug/ml | 0.00          |
| System Monitoring Compounds |       |       |          |          |       |               |
| 2) Tripropylphosphate       | 6.49  | 99    | 80111    | 0.10     | ug/ml | 0.00          |
| Spiked Amount               | 2.500 | Range | 20 - 150 | Recovery | =     | 4.00%#        |
| Target Compounds            |       |       |          |          |       |               |
| 3) White Phosphorus         | 4.75  | 124   | 94630    | 0.10     | ug/ml | Ovalue<br>100 |

# Quantitation Report


Data File : H:\VOL1\GCMSDATA\J\121112\BJ001203.D  
 Acq On : 12 Nov 2012 15:29  
 Sample : P4-1  
 Misc : P4 BNA J HLM  
 MS Integration Params: RTEINT.P  
 Quant Time: Nov 12 15:55 2012


Vial: 32  
 Operator: HLM  
 Inst : BNA J  
 Multiplr: 1.00

Instrument :  
 BNA\_J  
 LabSampleId :  
 P4-1

Quant Results File: BJ111212.FRES

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)  
 Title : P4 by SOP M.5  
 Last Update : Mon Nov 12 15:55:37 2012  
 Response via : Initial Calibration

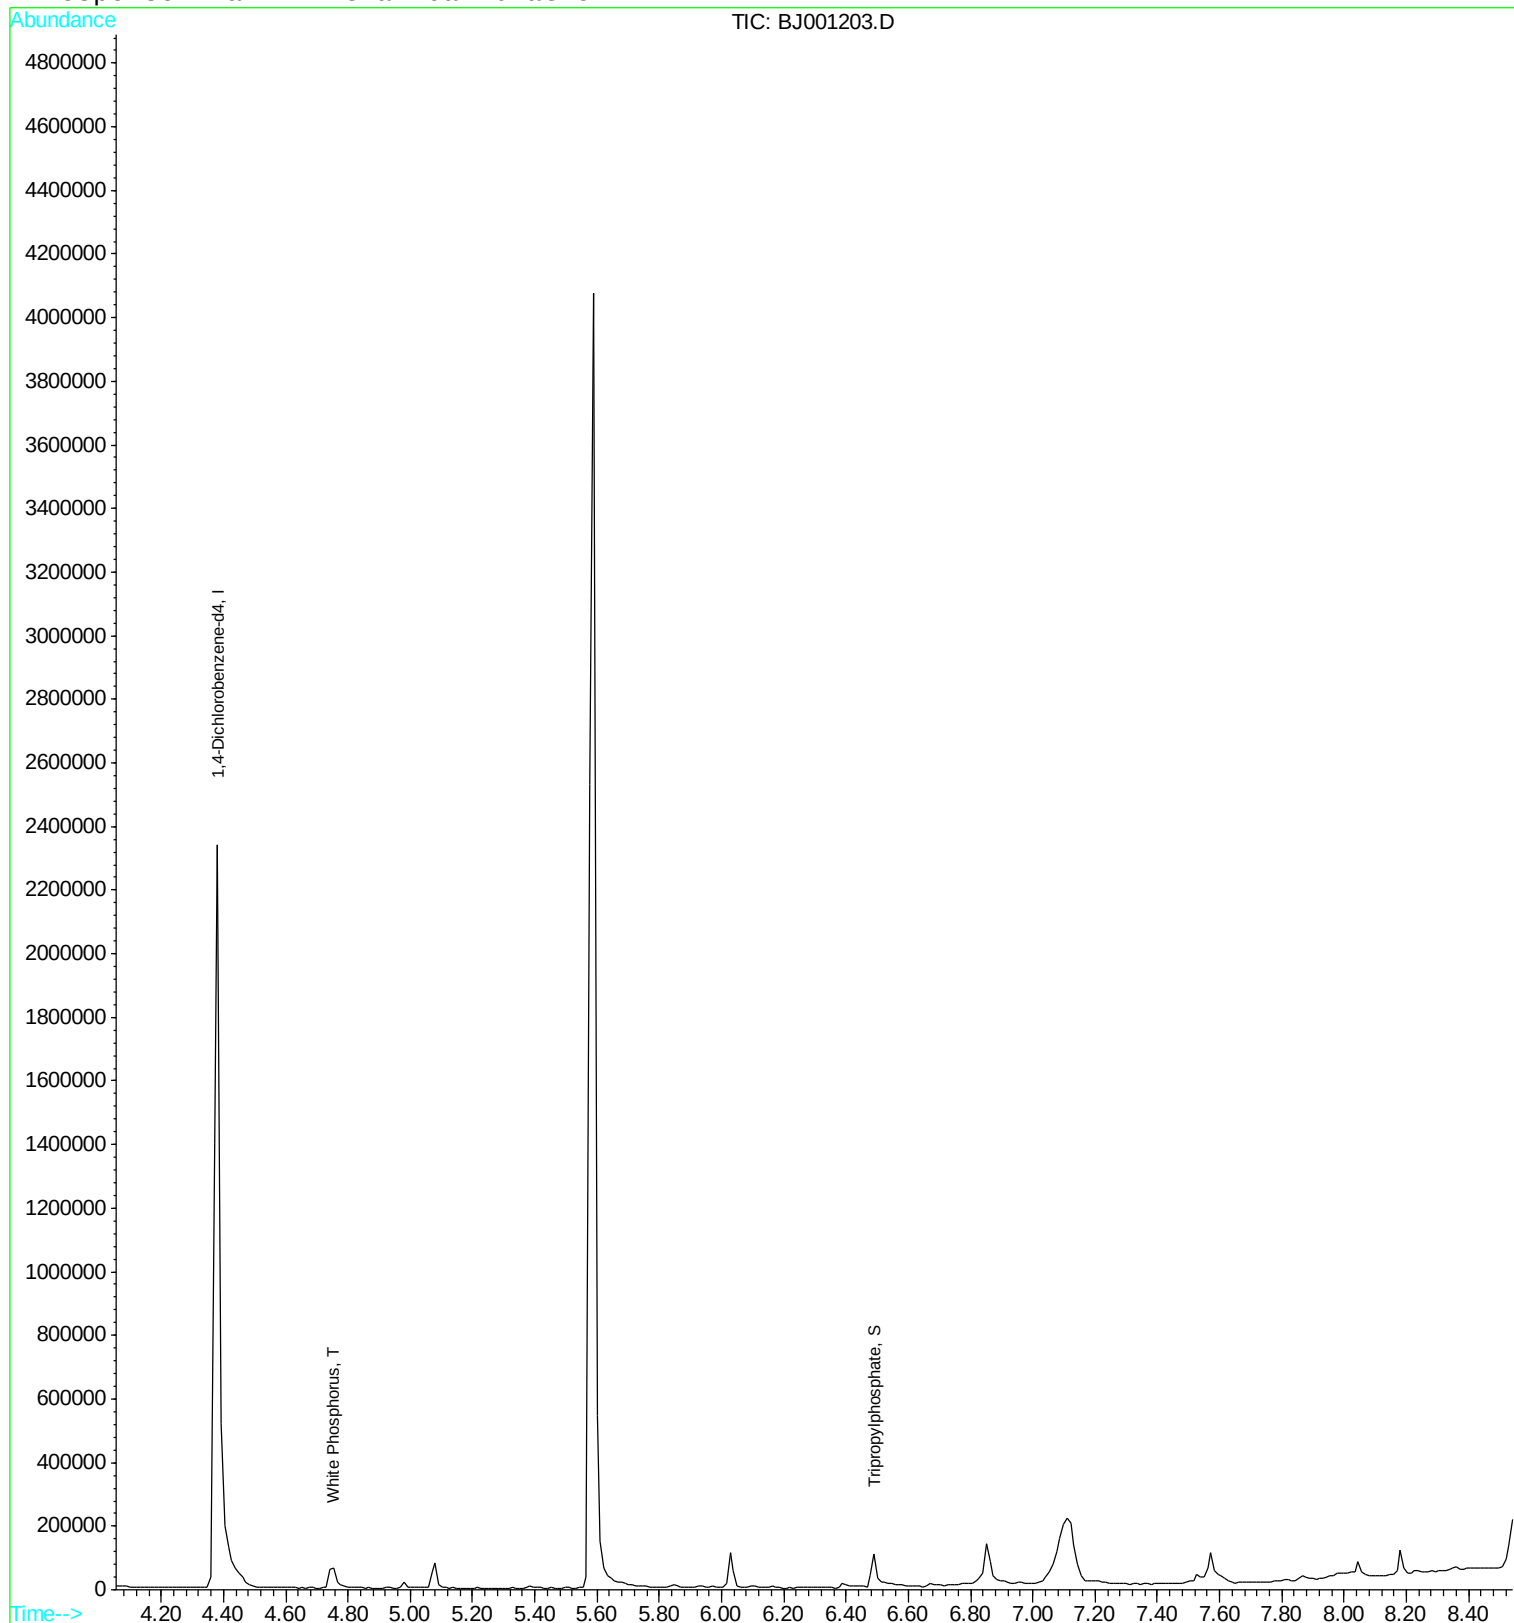

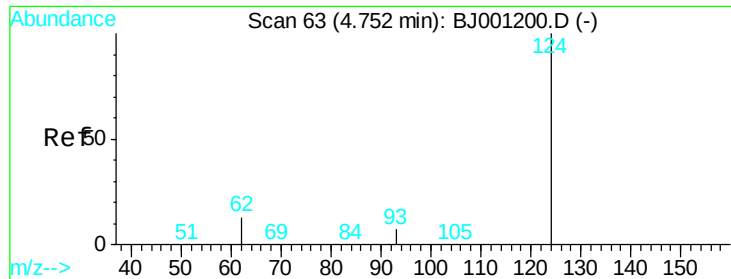

#3

White Phosphorus

Concen: 0.10 ug/ml

RT: 4.75 min Scan# 63

Delta R.T. 0.00 min

Lab File: BJ001203.D

Acq: 12 Nov 2012 15:29

Instrument :

BNA\_J

LabSampleId :

P4-1


Tgt Ion:124 Resp: 94630

Ion Ratio Lower Upper

124 100

93 7.1 0.0 27.3

62 16.0 0.0 35.9

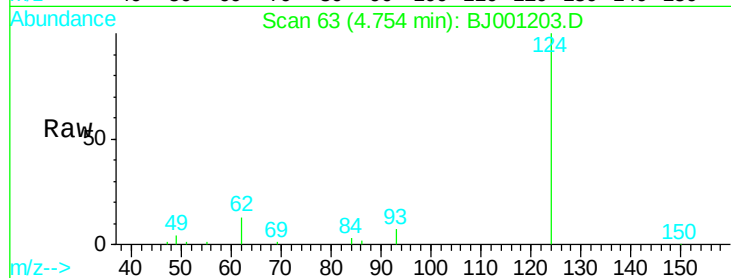

Abundance

Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

