

Data File : H:\VOL1\GCMSDATA\J\121112\BJ001221.D
Acq On : 12 Nov 2012 19:35
Sample : D4468-03
Misc : WATER LOD BNA J HLM
MS Integration Params: RTEINT.P
Quant Time: Nov 13 14:20 2012

Vial: 42
Operator: HLM
Inst : BNA J
Multiplr: 1.00

Instrument :
BNA_J
ClientSampleId :
LOD Water 2012-4

Quant Results File: BJ111212.P

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)
Title : P4 by SOP M.5
Last Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration
DataAcq Meth : P4

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.40	150	674514	2.50	ug/ml	0.02
System Monitoring Compounds						
2) Tripropylphosphate	6.51	99	1315505	2.42	ug/ml	0.02
Spiked Amount	2.500	Range	20 - 150	Recovery	=	96.80%
Target Compounds						
3) White Phosphorus	4.77	124	22664	0.04	ug/ml	Ovalue 89

Quantitation Report

Data File : H:\VOL1\GCMSDATA\J\121112\BJ001221.D

Vial: 42

Acq On : 12 Nov 2012 19:35

Operator: HLM

Sample : D4468-03

Inst : BNA J

Misc : WATER LOD BNA J HLM

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 13 14:20 2012

Quant Results File: BJ111212.P

Instrument :

BNA_J

ClientSampleId :


LOD Water 2012-4




Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)

Title : P4 by SOP M.5

Last Update : Mon Nov 12 15:57:53 2012

Response via : Initial Calibration

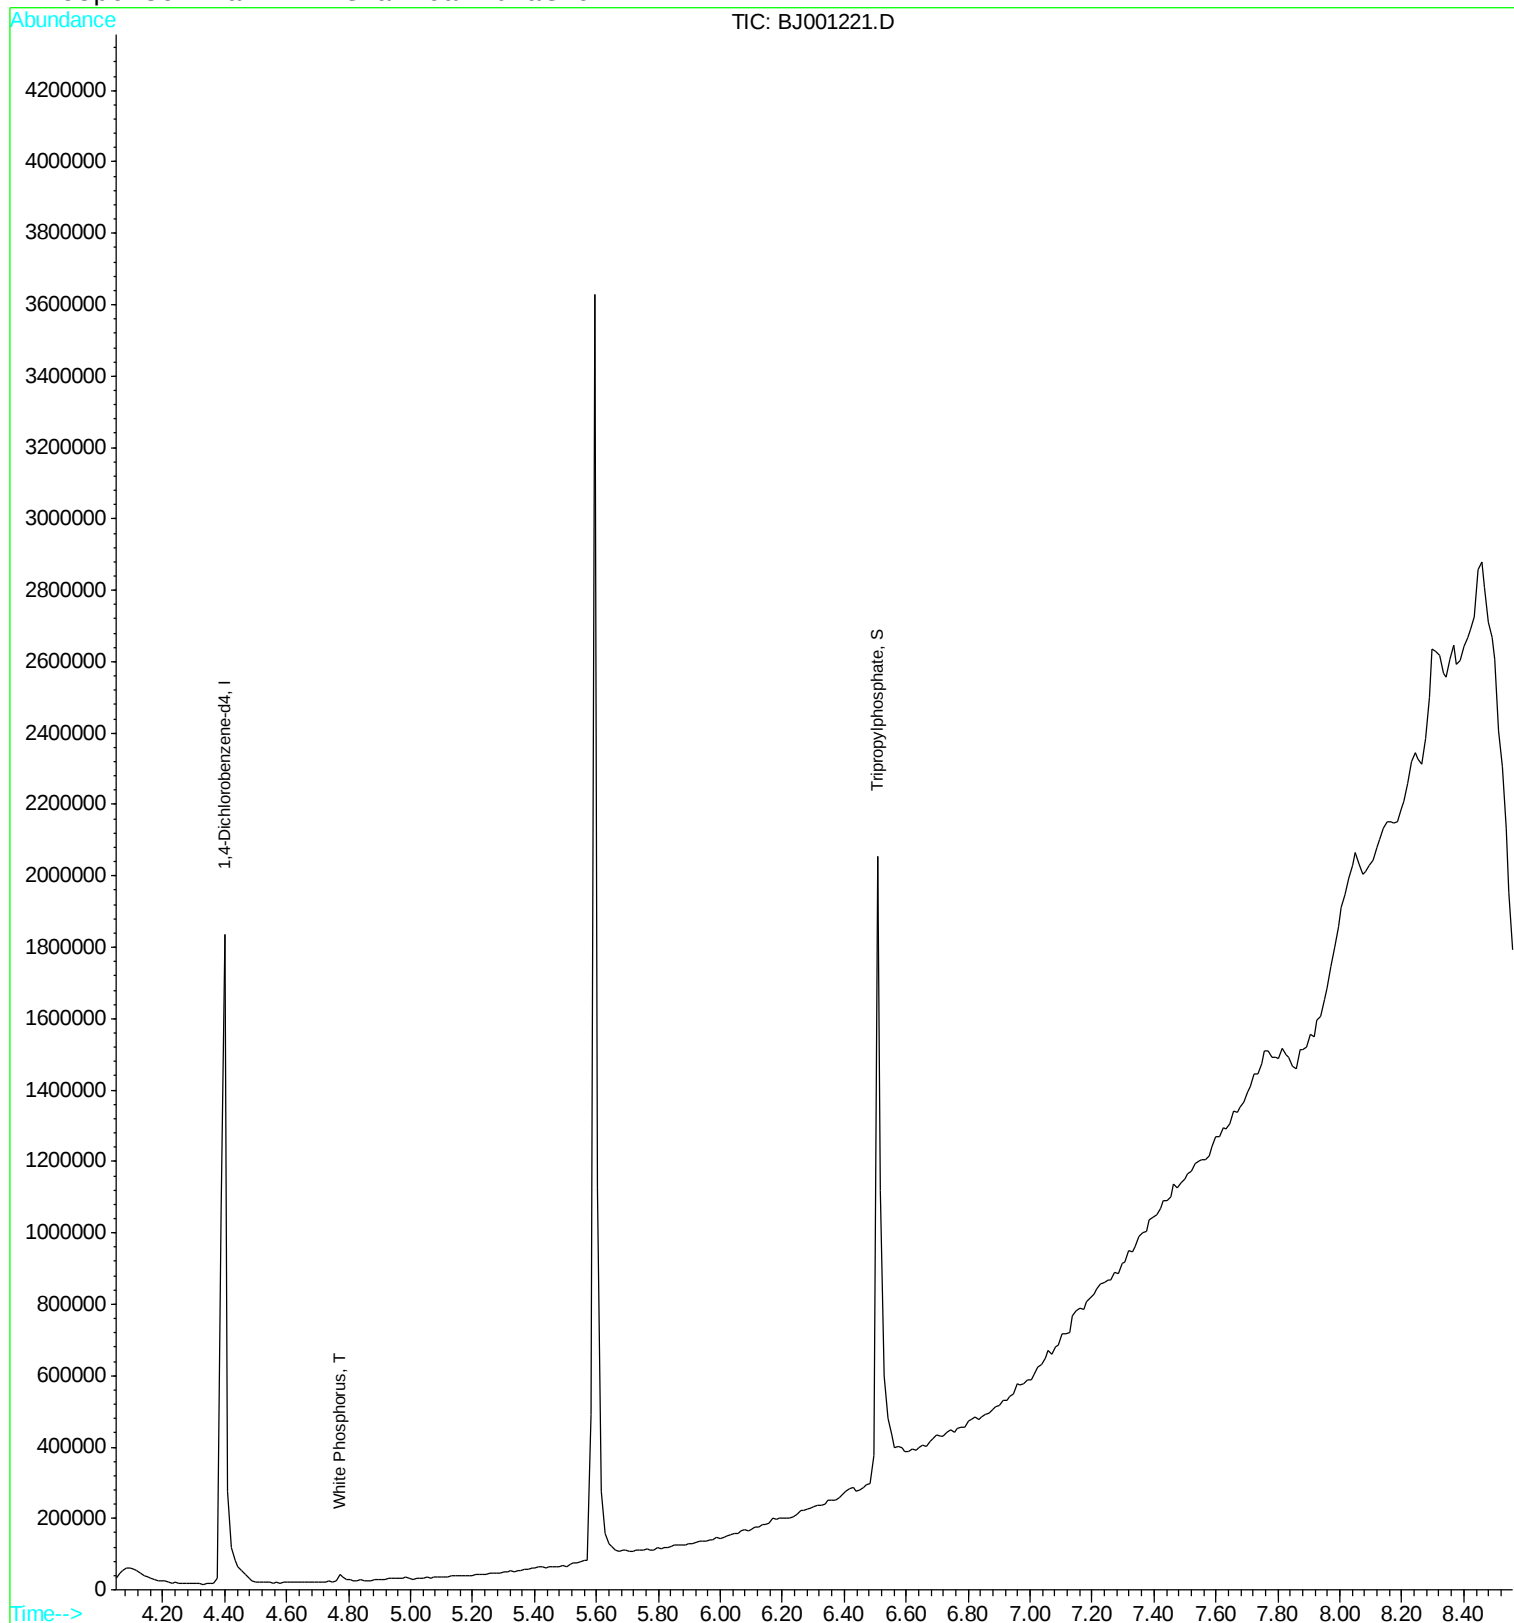

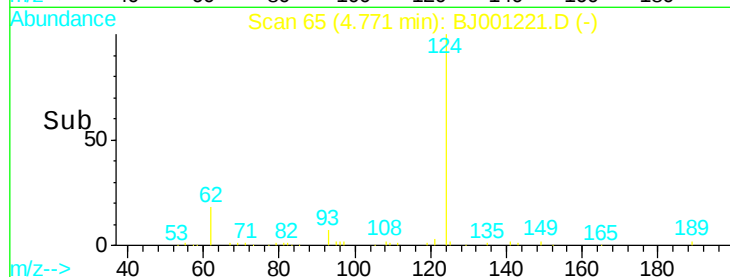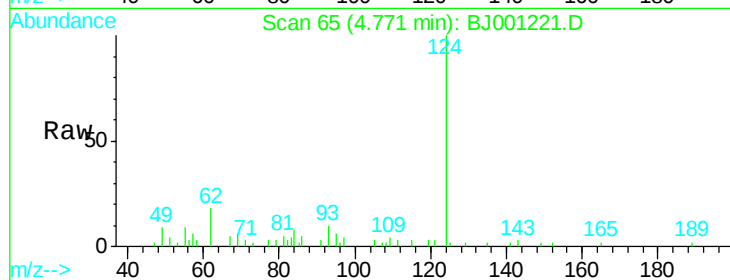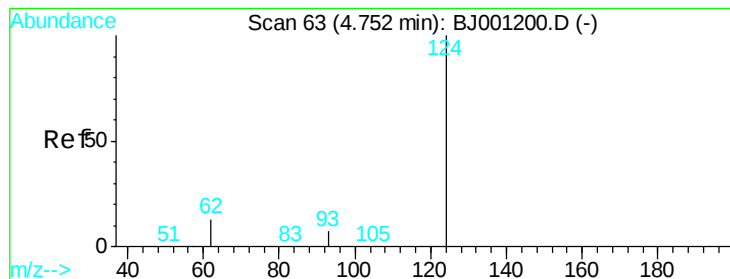

#3

White Phosphorus

Concen: 0.04 ug/ml

RT: 4.77 min Scan# 65

Delta R.T. 0.02 min

Lab File: BJ001221.D

Acq: 12 Nov 2012 19:35

Instrument :

BNA_J

ClientSampleId :

LOD Water 2012-4

Tgt Ion:124 Resp: 22664

Ion Ratio Lower Upper

124 100

93 19.3 0.0 27.3

62 16.1 0.0 35.9

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

