

Data File : H:\VOL1\GCMSDATA\J\121112\BJ001222.D
Acq On : 12 Nov 2012 19:48
Sample : D4468-04
Misc : WATER LOO BNA J HLM
MS Integration Params: RTEINT.P
Quant Time: Nov 13 14:20 2012

Vial: 43
Operator: HLM
Inst : BNA J
Multiplr: 1.00

Instrument :
BNA_J
ClientSampleId :
LOO Water 2012-04

Quant Results File: BJ111212.PES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)
Title : P4 by SOP M.5
Last Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration
DataAcq Meth : P4

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.40	150	675309	2.50	ug/ml	0.02
System Monitoring Compounds						
2) Tripropylphosphate	6.51	99	1417860	2.60	ug/ml	0.02
Spiked Amount	2.500	Range	20 - 150	Recovery	=	104.00%
Target Compounds						
3) White Phosphorus	4.77	124	91860	0.14	ug/ml	Ovalue 99

Data File : H:\VOL1\GCMSDATA\J\121112\BJ001222.D

Vial: 43

Acq On : 12 Nov 2012 19:48

Operator: HLM

Sample : D4468-04

Inst : BNA J

Misc : WATER LOO BNA J HLM

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 13 14:20 2012

Quant Results File: BJ111212.PES

Instrument :

BNA_J

ClientSampleId :


LOO Water 2012-04


Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)

Title : P4 by SOP M.5

Last Update : Mon Nov 12 15:57:53 2012

Response via : Initial Calibration

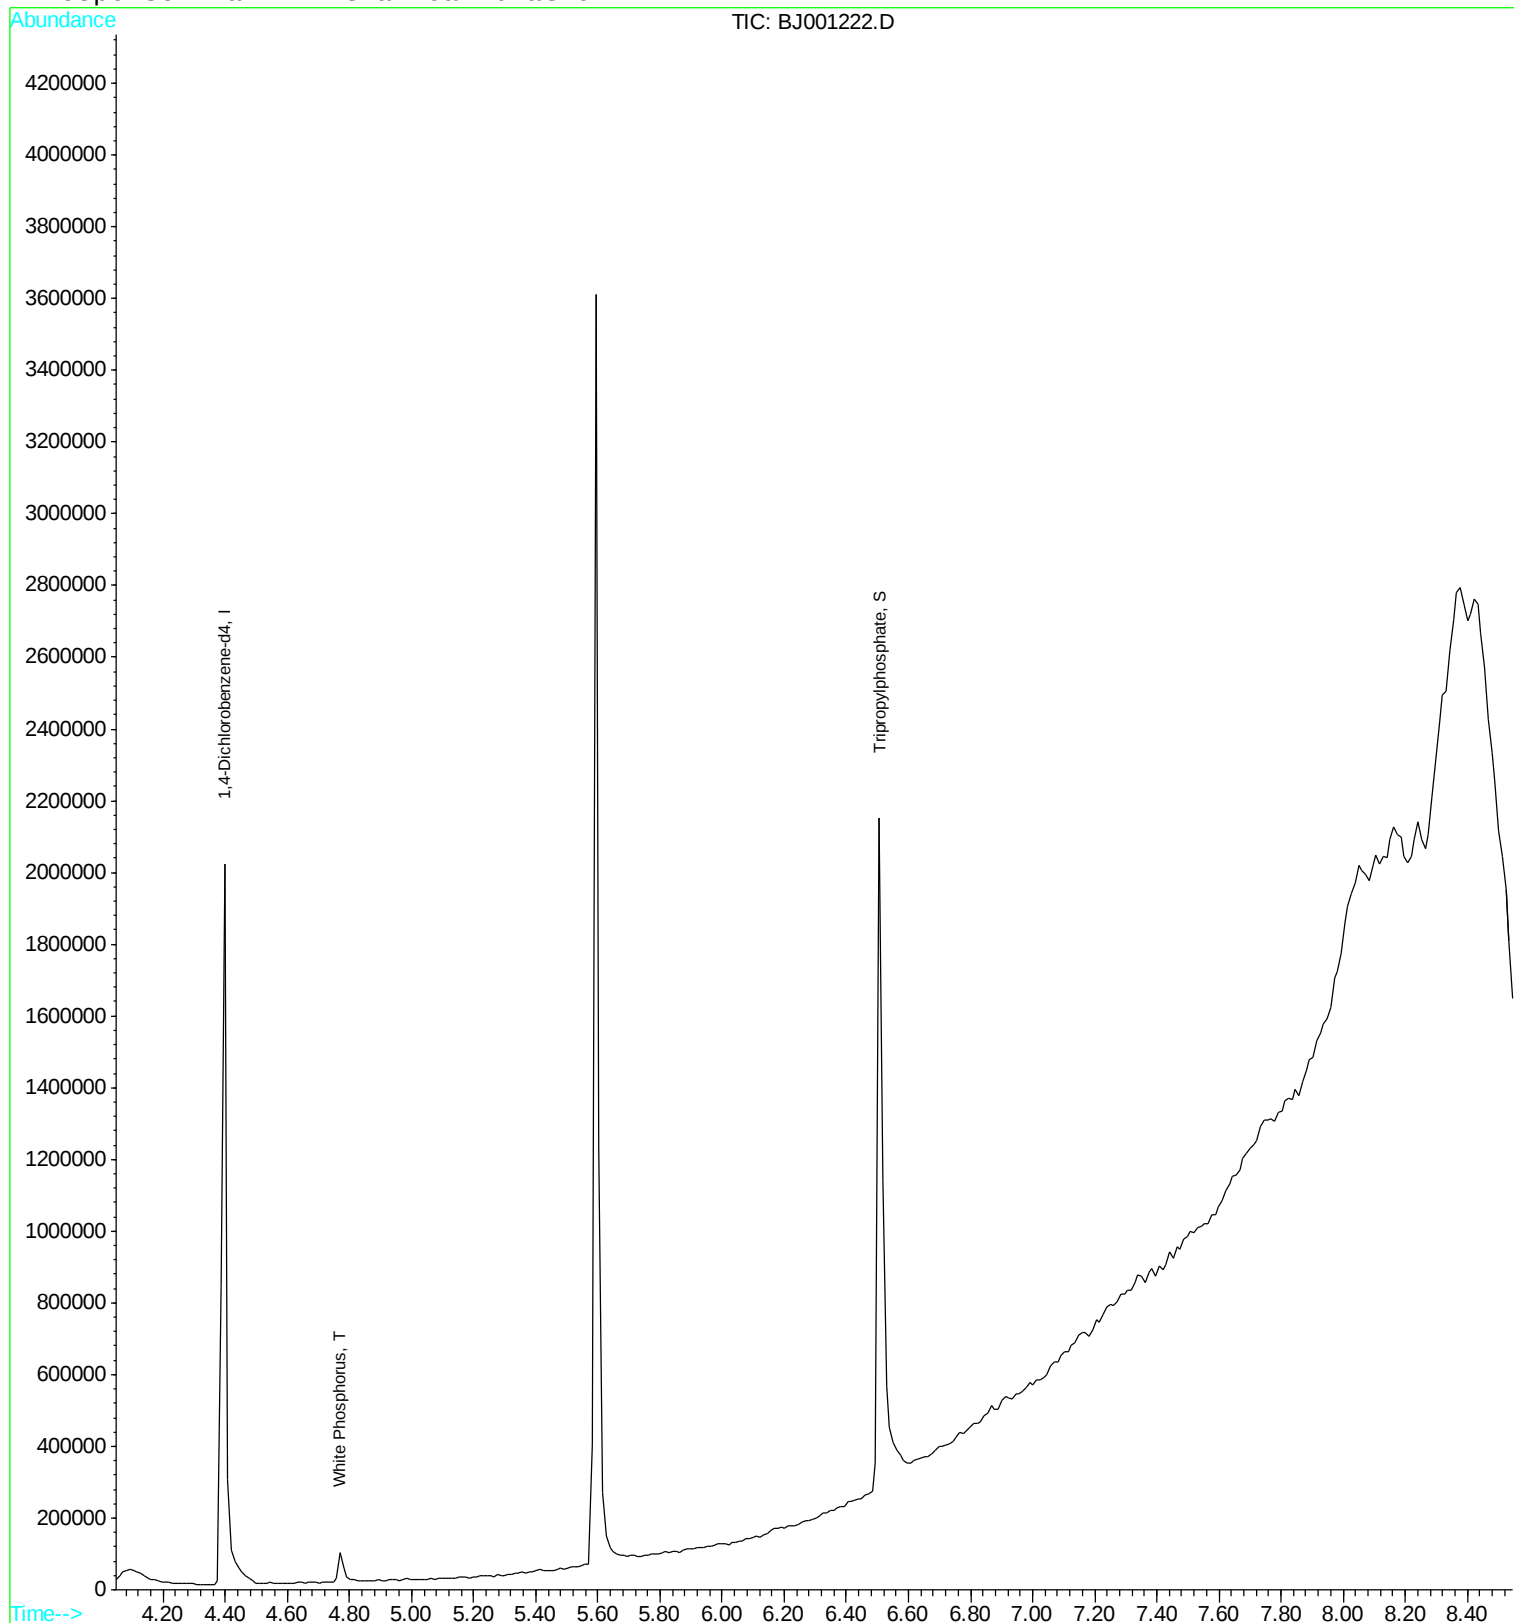

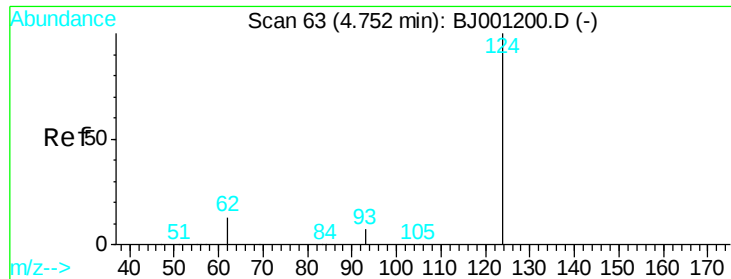

#3

White Phosphorus

Concen: 0.14 ug/ml

RT: 4.77 min Scan# 65

Delta R.T. 0.02 min

Lab File: BJ001222.D


Acq: 12 Nov 2012 19:48

Instrument :

BNA_J

ClientSampleId :

LOQ Water 2012-04

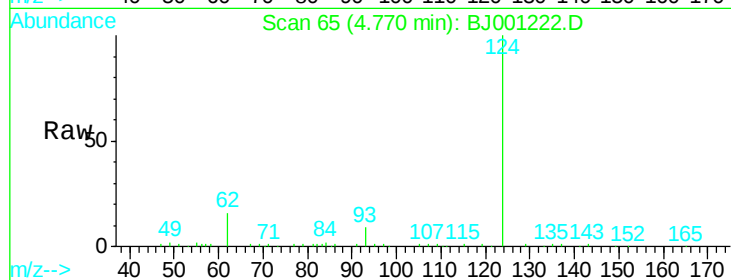


Tgt Ion:124 Resp: 91860

Ion Ratio Lower Upper

124 100

93 7.4 0.0 27.3

62 15.4 0.0 35.9

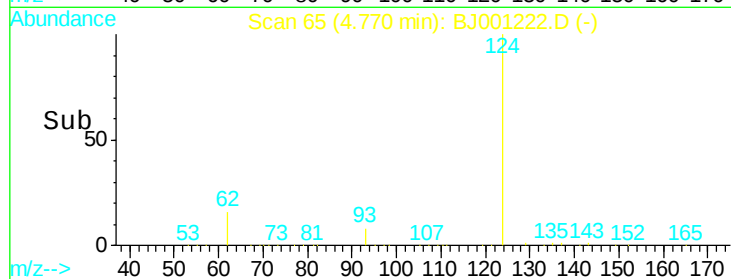

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

