

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001199.D
Acq On : 12 Nov 2012 14:37
Operator : HLM
Sample : P4-5
Misc : P4 BNA_J HLM
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-5

Quant Time: Nov 19 00:19:46 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:55:37 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.38	150	821326	2.50	ug/ml	0.00

System Monitoring Compounds
2) Tripropylphosphate 6.49 99 1617532 2.33 ug/ml 0.00
Spiked Amount 2.500 Range 20 - 150 Recovery = 93.20%


Target Compounds					Qvalue
3) White Phosphorus	4.75	124	1908597	2.46	ug/ml 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001199.D
Acq On : 12 Nov 2012 14:37
Operator : HLM
Sample : P4-5
Misc : P4 BNA_J HLM
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-5

Quant Time: Nov 19 00:19:46 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:55:37 2012
Response via : Initial Calibration

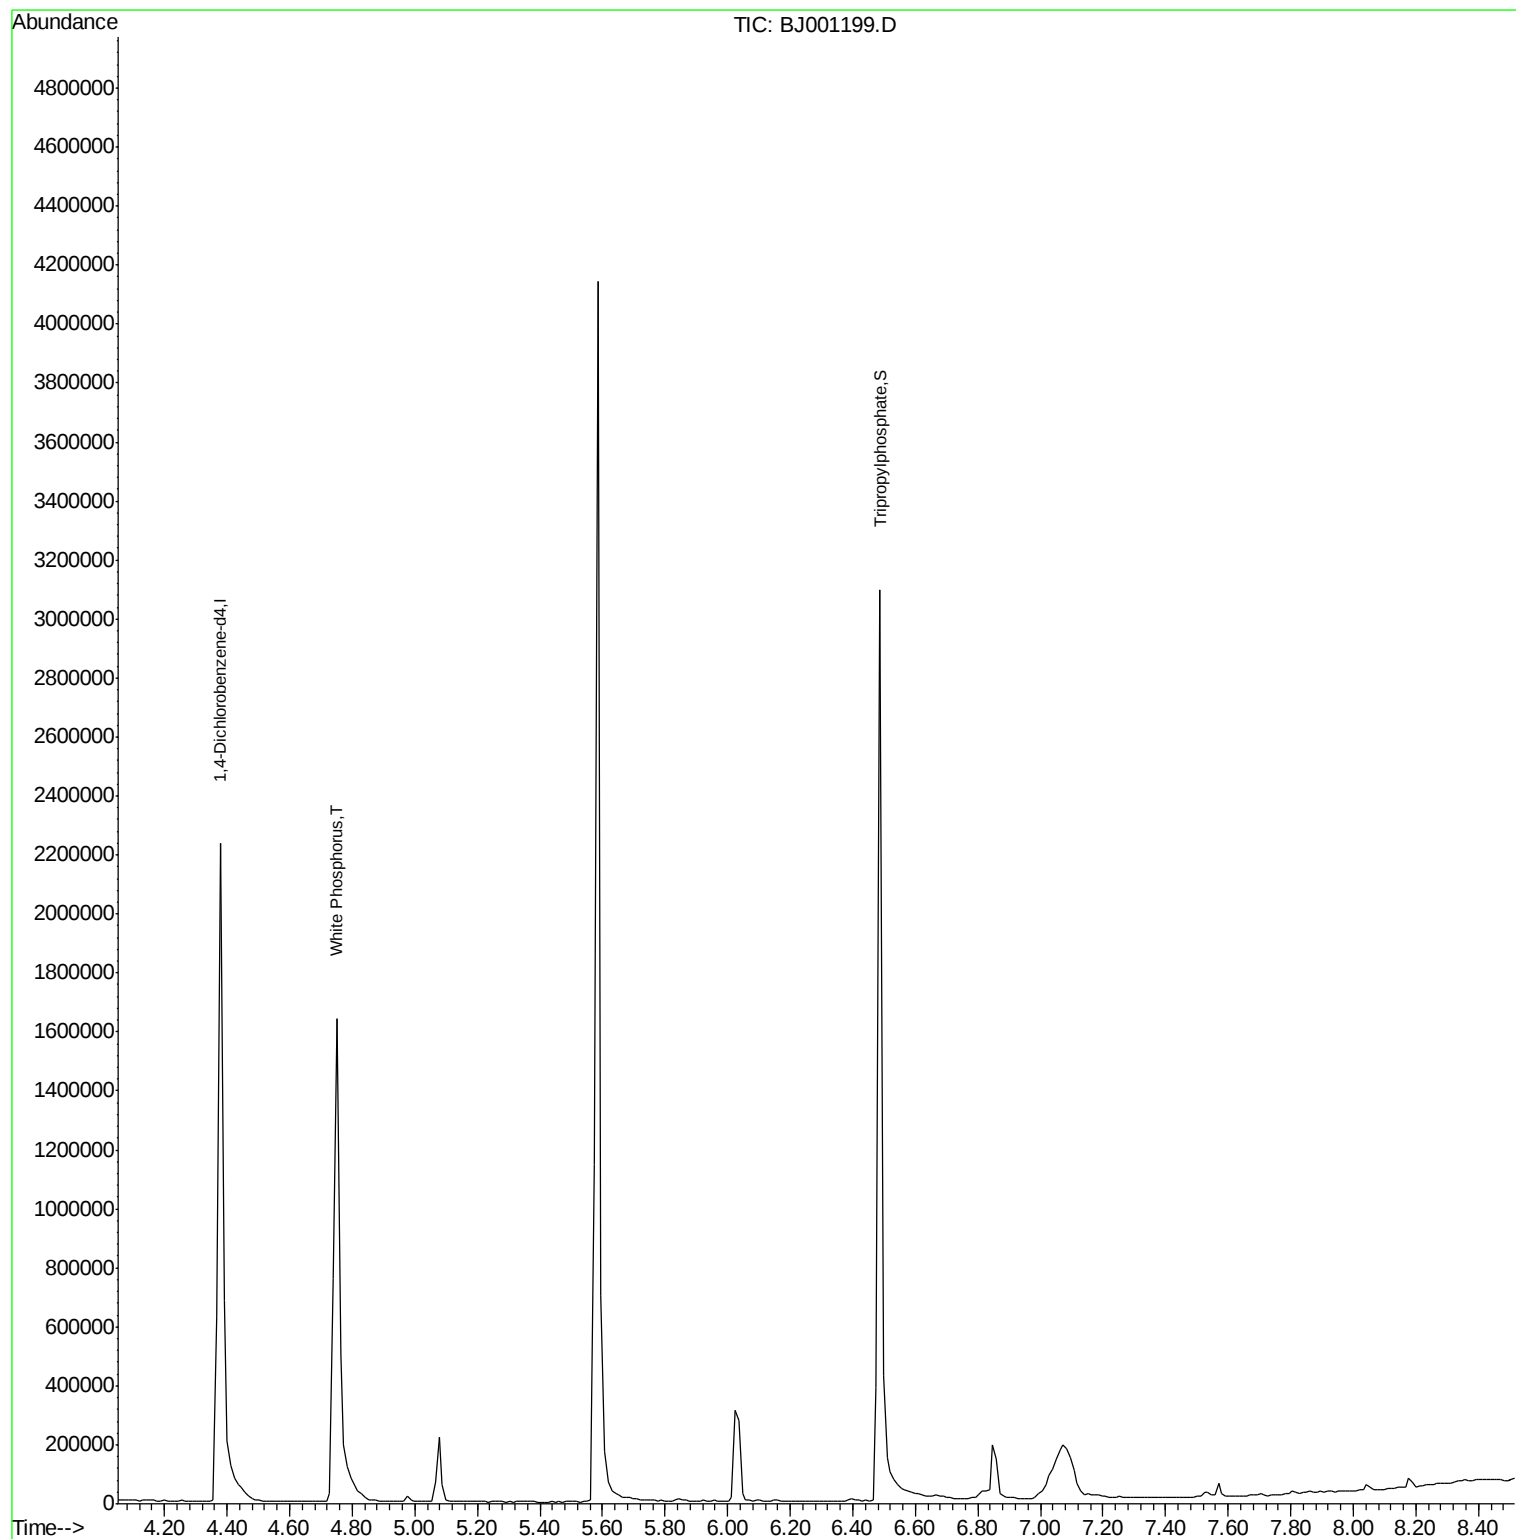

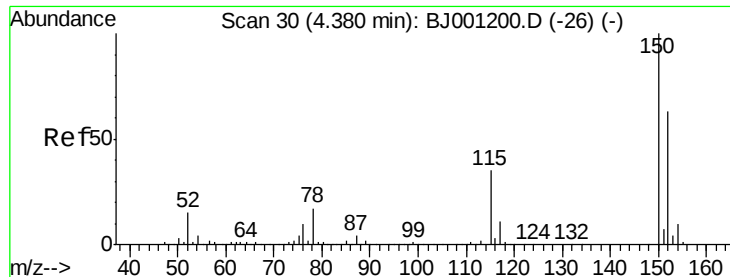


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.38 min Scan# 30
Delta R.T. -0.00 min
Lab File: BJ001199.D
Acq: 12 Nov 2012 14:37

Instrument :
BNA_J
LabSampleId :
P4-5

Tgt Ion: 150 Resp: 821326
Ion Ratio Lower Upper
150 100
152 63.4 43.1 83.1

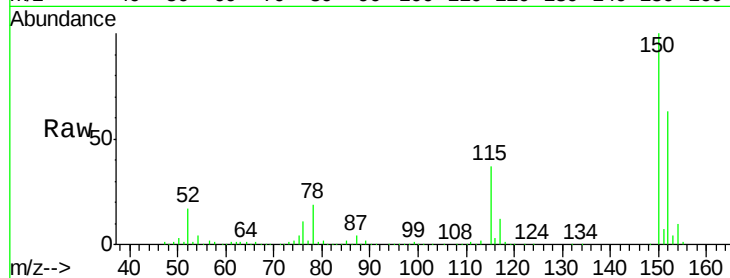


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

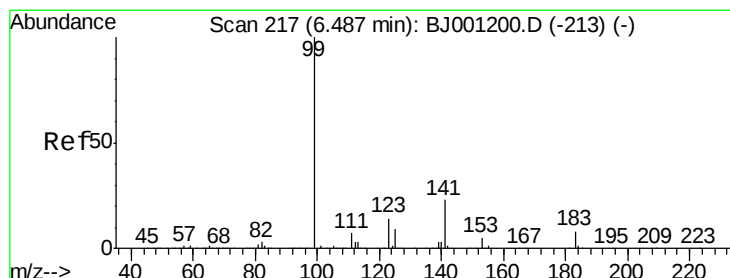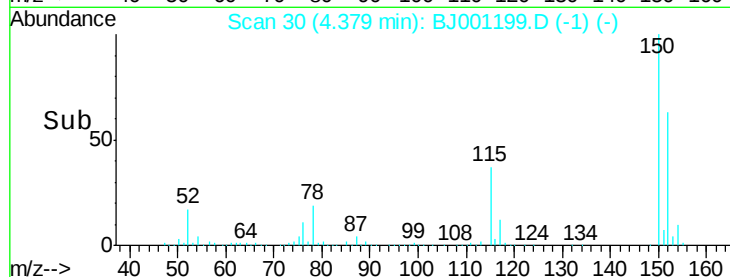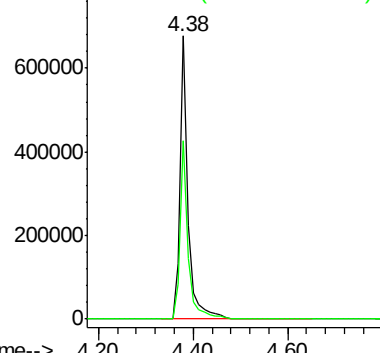



#2


Tripropylphosphate
Concen: 2.33 ug/ml
RT: 6.49 min Scan# 217
Delta R.T. -0.00 min
Lab File: BJ001199.D
Acq: 12 Nov 2012 14:37

Tgt Ion: 99 Resp: 1617532
Ion Ratio Lower Upper
99 100
141 21.2 0.8 40.8

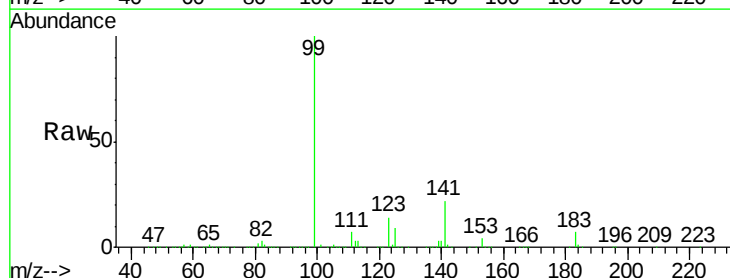

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

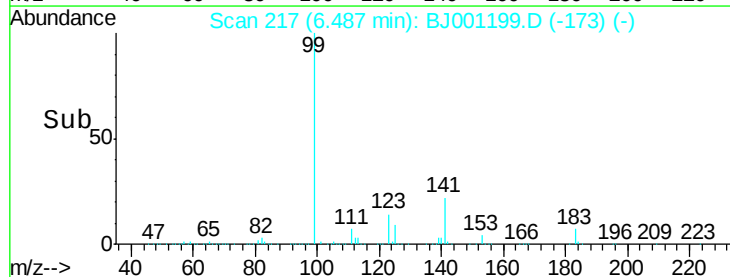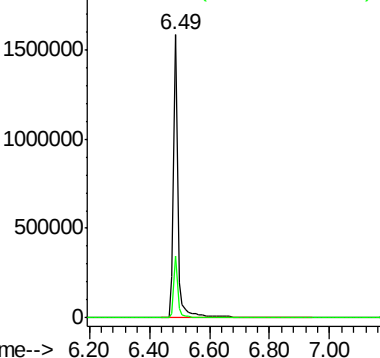

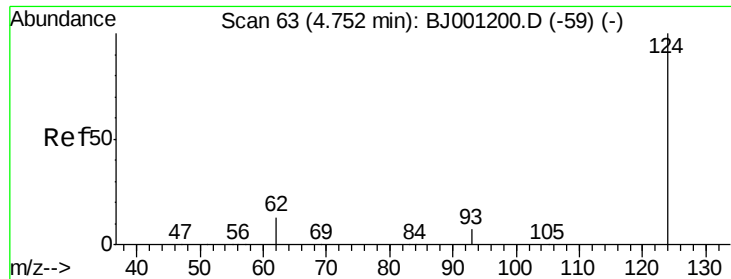

#3
 White Phosphorus
 Concen: 2.46 ug/ml
 RT: 4.75 min Scan# 63
 Delta R.T. -0.00 min
 Lab File: BJ001199.D
 Acq: 12 Nov 2012 14:37

Instrument :
 BNA_J
 LabSampleId :
 P4-5

Tgt Ion:124 Resp: 1908597

Ion	Ratio	Lower	Upper
124	100		
93	7.3	0.0	27.3
62	16.0	0.0	35.9

