

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001201.D
Acq On : 12 Nov 2012 15:03
Operator : HLM
Sample : P4-3
Misc : P4 BNA_J HLM
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-3

Quant Time: Nov 15 13:38:16 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:55:37 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.38	150	895446	2.50	ug/ml	0.00

System Monitoring Compounds
2) Tripropylphosphate 6.48 99 356097 0.47 ug/ml 0.00
Spiked Amount 2.500 Range 20 - 150 Recovery = 18.80%#


Target Compounds					Qvalue
3) White Phosphorus	4.75	124	419907	0.50 ug/ml	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001201.D
Acq On : 12 Nov 2012 15:03
Operator : HLM
Sample : P4-3
Misc : P4 BNA_J HLM
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-3

Quant Time: Nov 15 13:38:16 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:55:37 2012
Response via : Initial Calibration

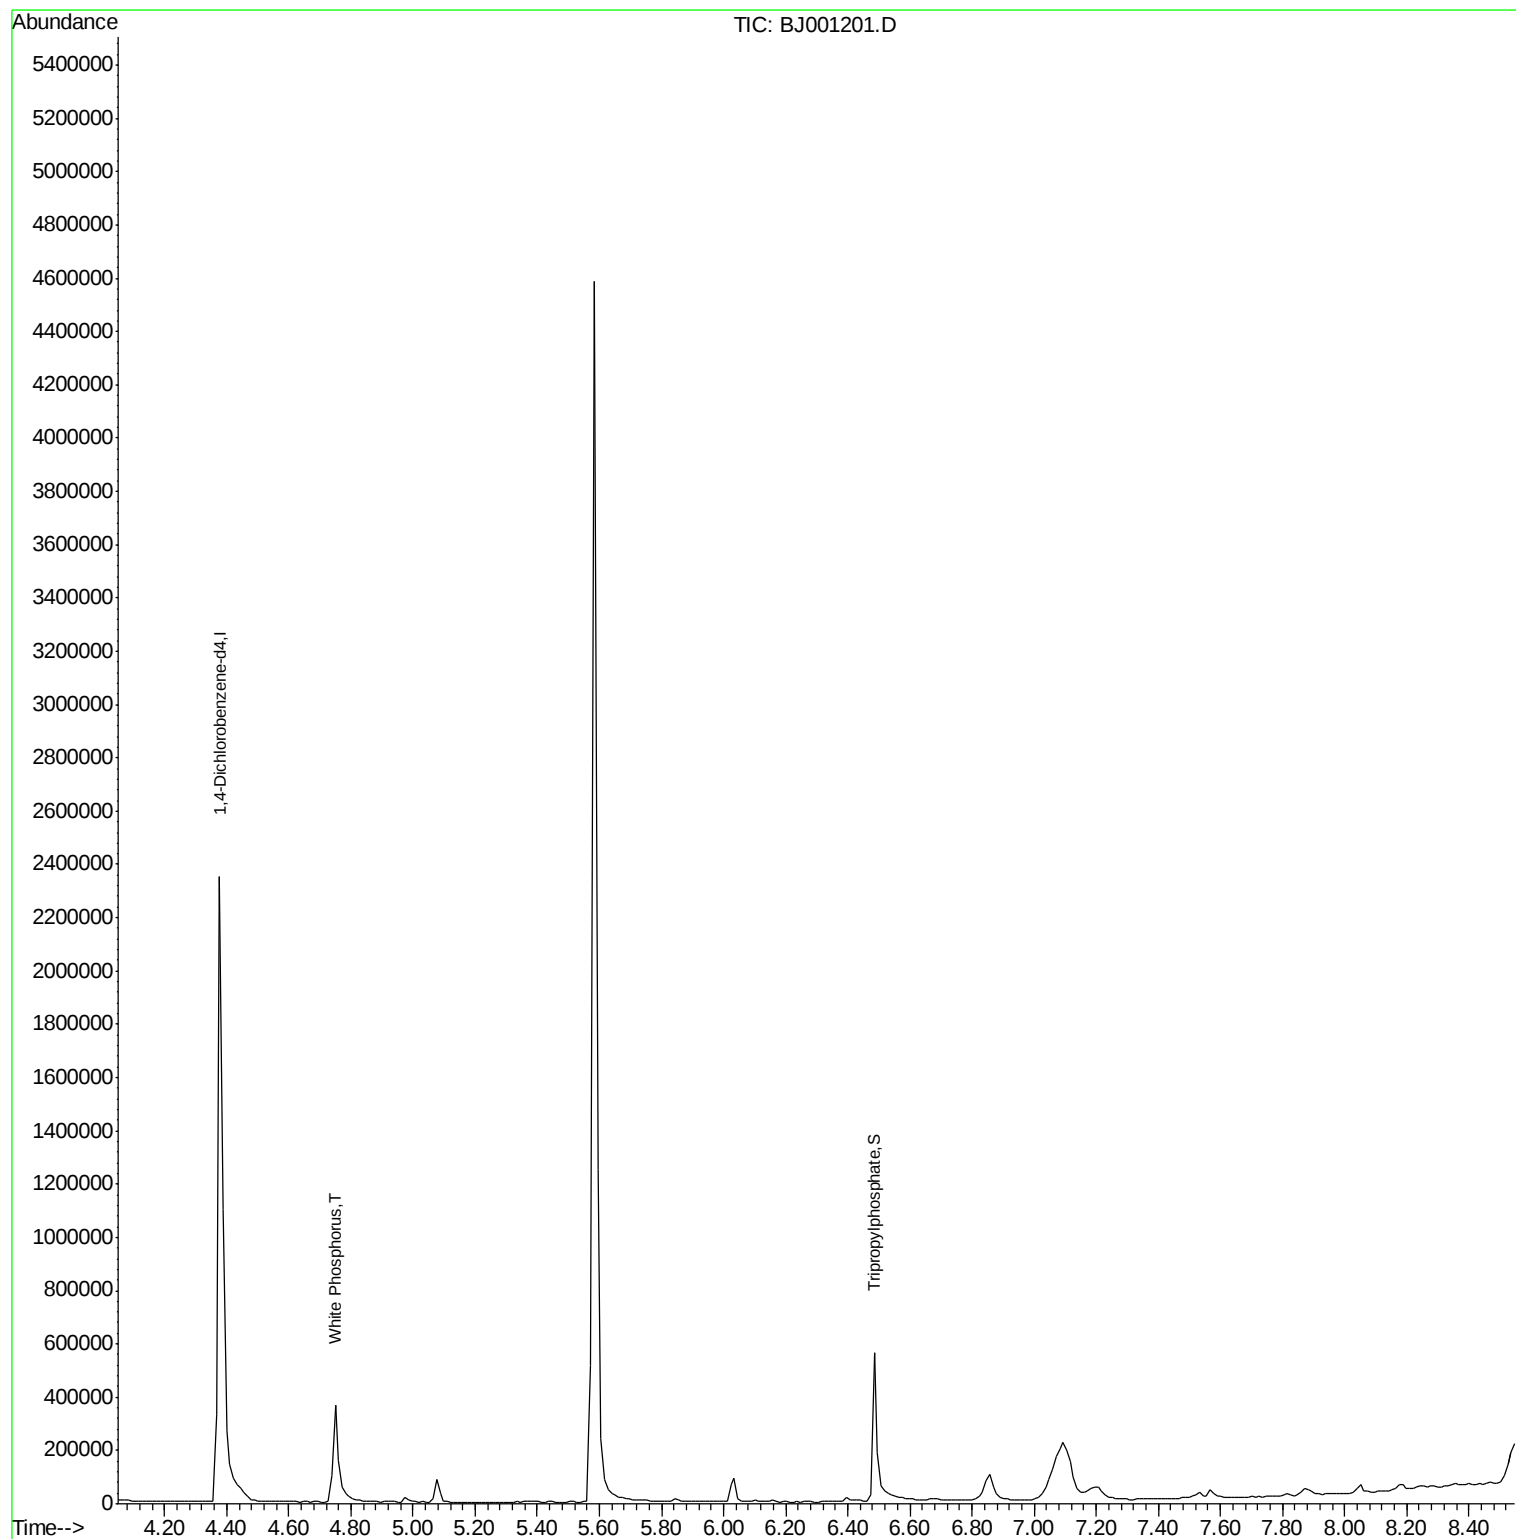




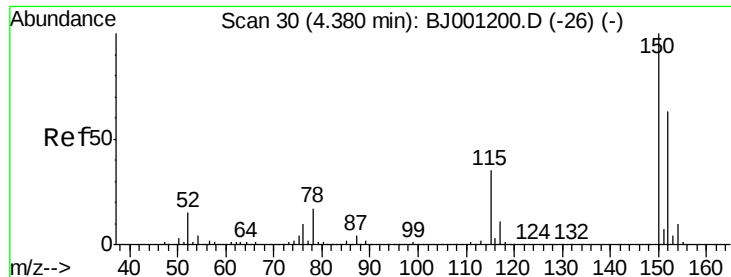


#1

1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.38 min Scan# 30
Delta R.T. -0.00 min
Lab File: BJ001201.D
Acq: 12 Nov 2012 15:03

Instrument :
BNA_J
LabSampleId :
P4-3




Tgt Ion:150 Resp: 895446
Ion Ratio Lower Upper
150 100
152 63.4 43.1 83.1

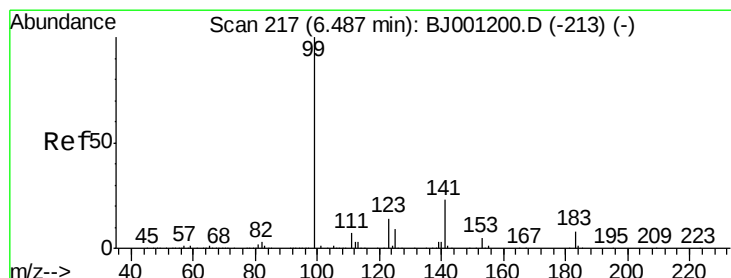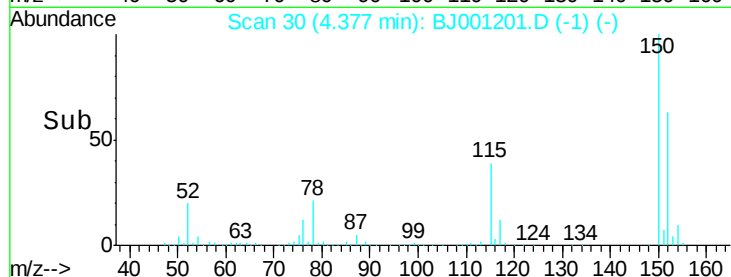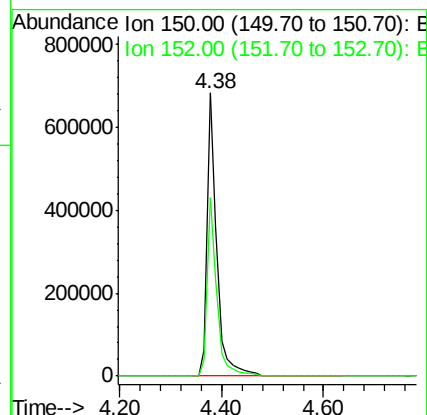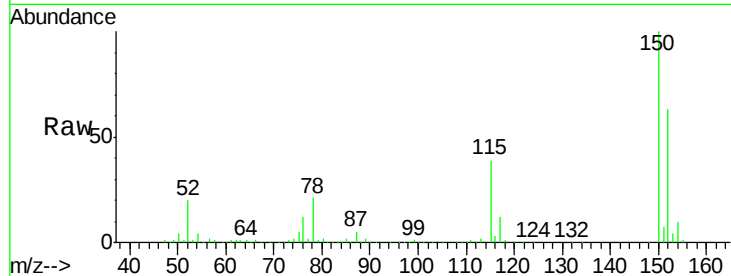


#2

Tripropylphosphate
Concen: 0.47 ug/ml
RT: 6.48 min Scan# 217
Delta R.T. -0.00 min
Lab File: BJ001201.D
Acq: 12 Nov 2012 15:03

Tgt Ion: 99 Resp: 356097
Ion Ratio Lower Upper
99 100
141 20.0 0.8 40.8

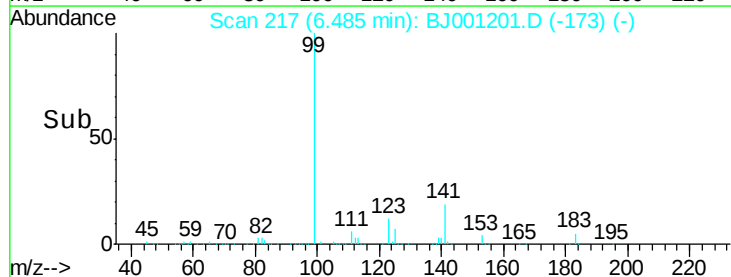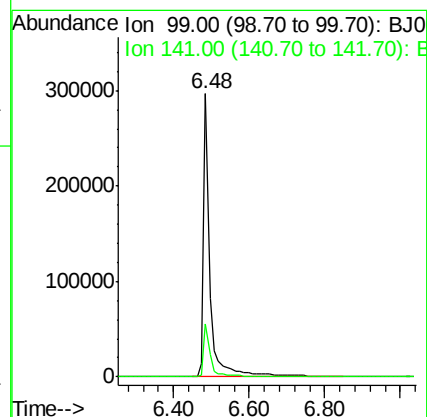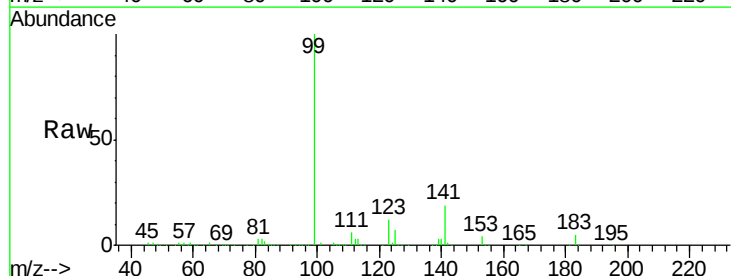

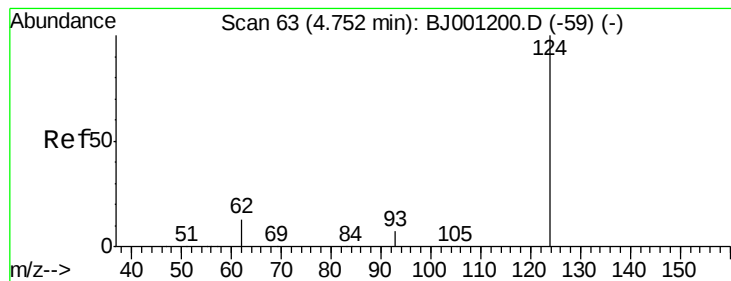

#3

White Phosphorus

Concen: 0.50 ug/ml

RT: 4.75 min Scan# 63

Delta R.T. -0.00 min

Lab File: BJ001201.D


Acq: 12 Nov 2012 15:03

Instrument :

BNA_J

LabSampleId :

P4-3

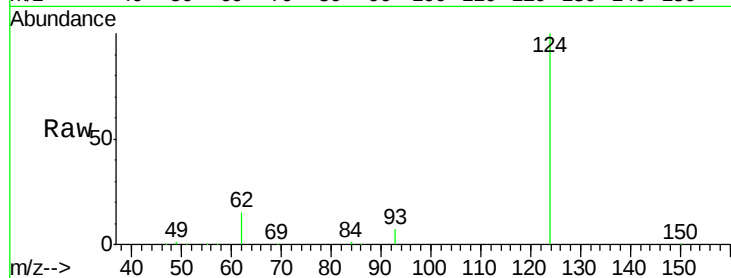


Tgt Ion:124 Resp: 419907

Ion Ratio Lower Upper

124 100

93 7.2 0.0 27.3

62 15.7 0.0 35.9

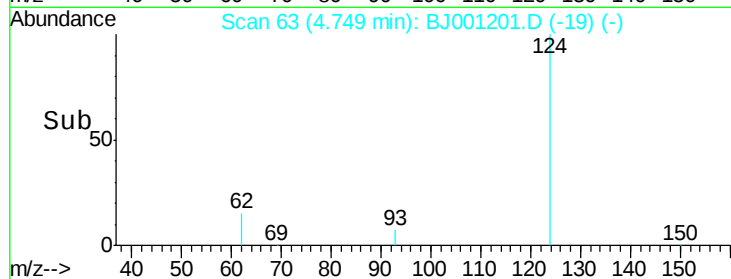

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

400000

300000

200000

100000

0

4.75

4.60 4.70 4.80 4.90 5.00

Time-->