

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001204.D
Acq On : 12 Nov 2012 15:42
Operator : HLM
Sample : P4-ICV
Misc : P4 BNA_J HLM
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-ICV

Quant Time: Nov 15 16:22:58 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:06 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.38	150	716493	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	0.00	99	0	0.00	ug/ml	
Spiked Amount	2.500	Range	20 - 150	Recovery	=	0.00%#

Target Compounds


					Qvalue
3) White Phosphorus	4.75	124	645521	0.95	ug/ml 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001204.D
Acq On : 12 Nov 2012 15:42
Operator : HLM
Sample : P4-ICV
Misc : P4 BNA_J HLM
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
P4-ICV

Quant Time: Nov 15 16:22:58 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:06 2012
Response via : Initial Calibration

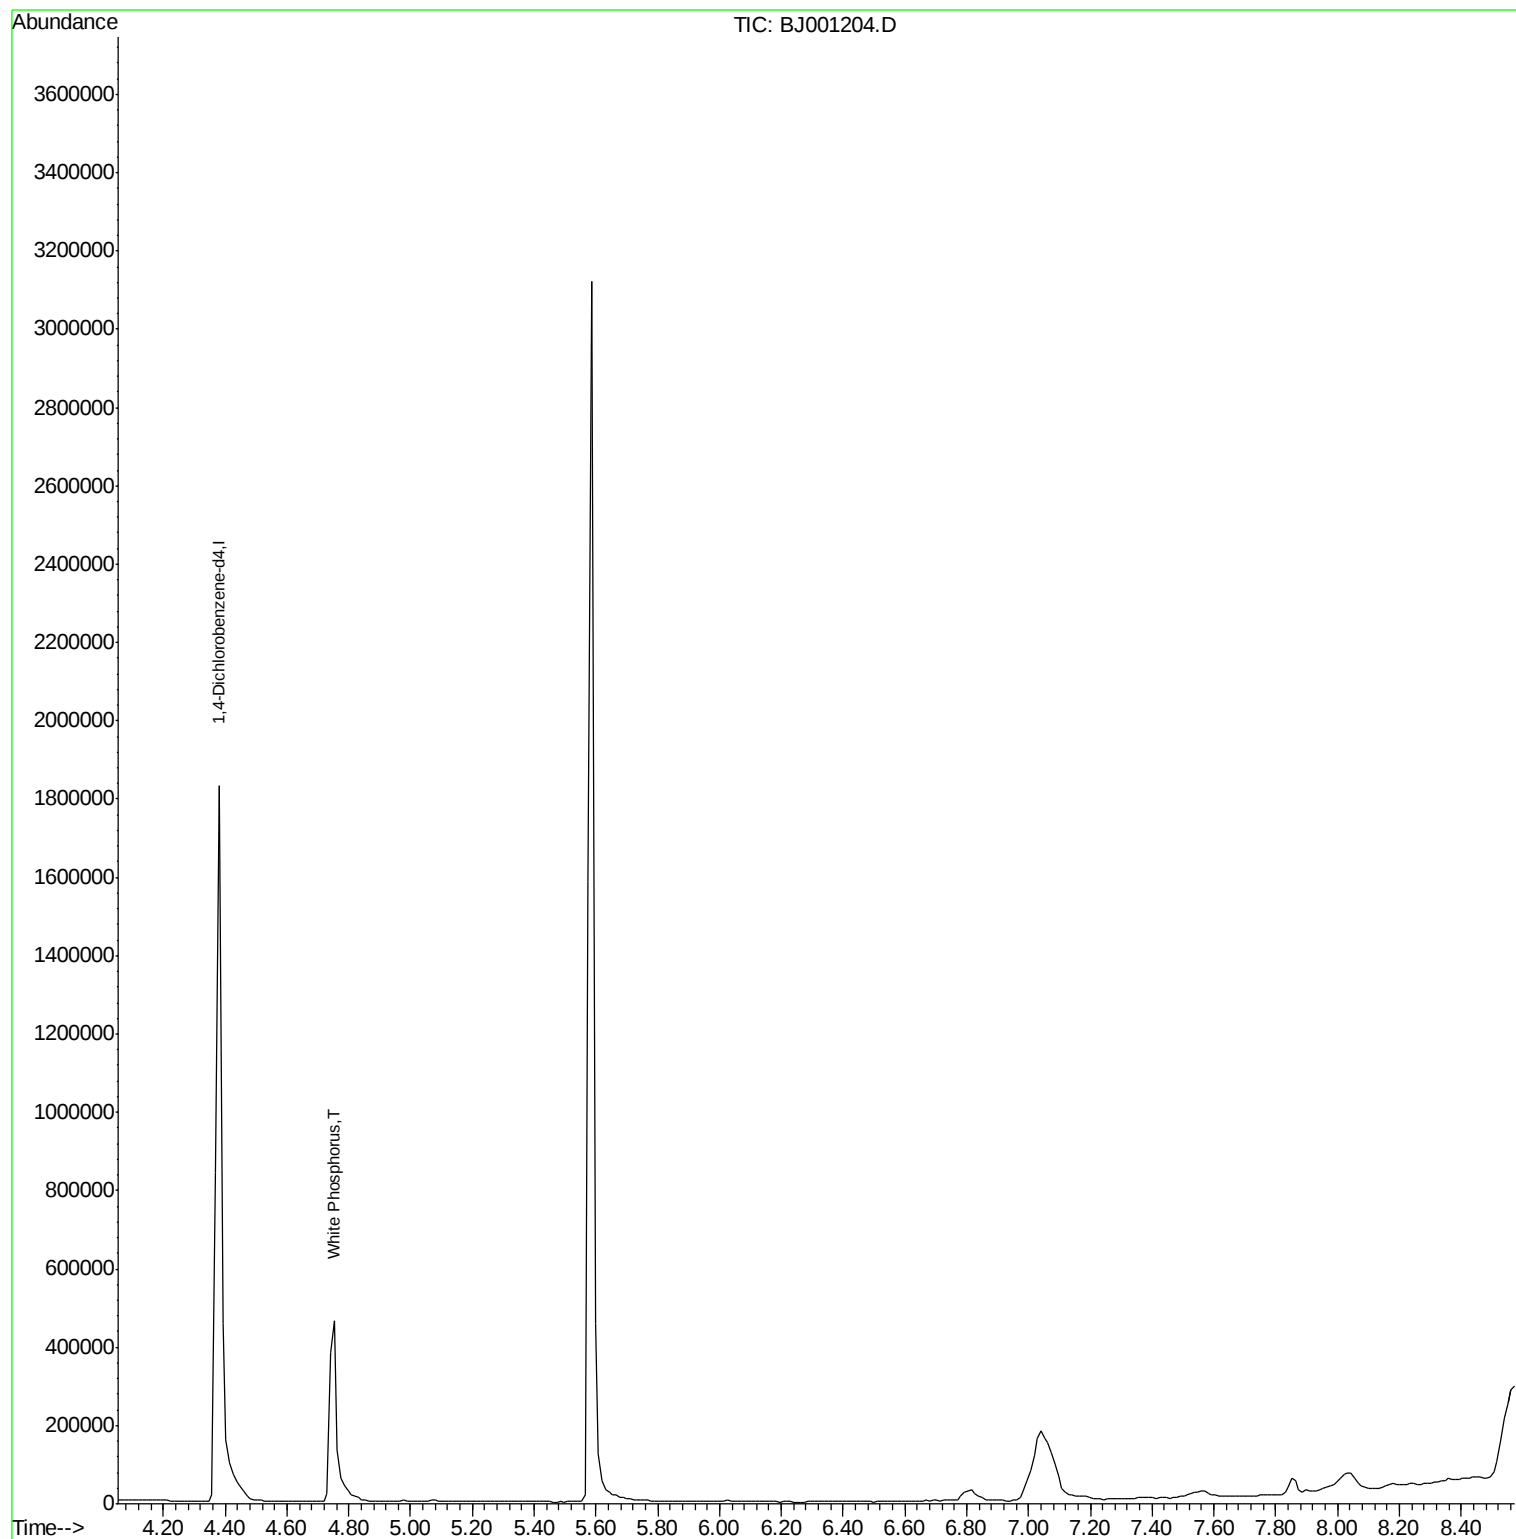

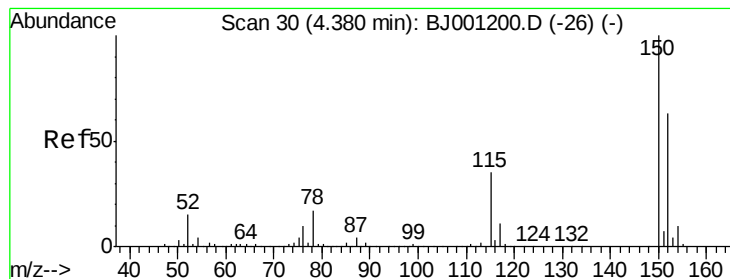


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.38 min Scan# 30
Delta R.T. 0.00 min
Lab File: BJ001204.D
Acq: 12 Nov 2012 15:42

Instrument :
BNA_J
ClientSampleId :
P4-ICV

Tgt Ion:150 Resp: 716493
Ion Ratio Lower Upper
150 100
152 63.8 43.1 83.1

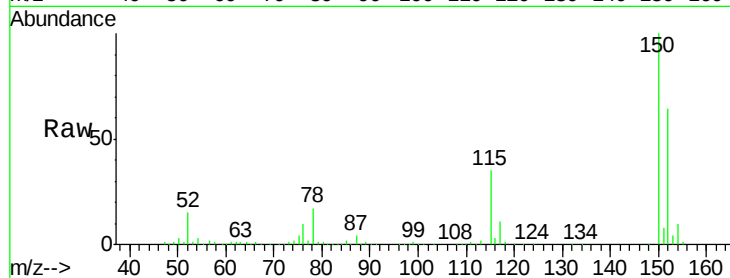

Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

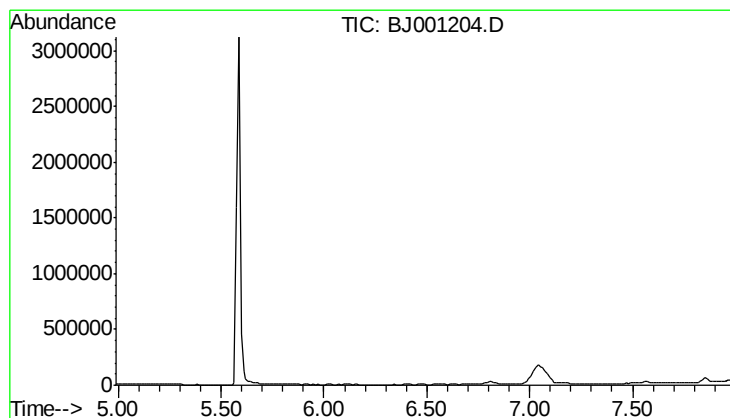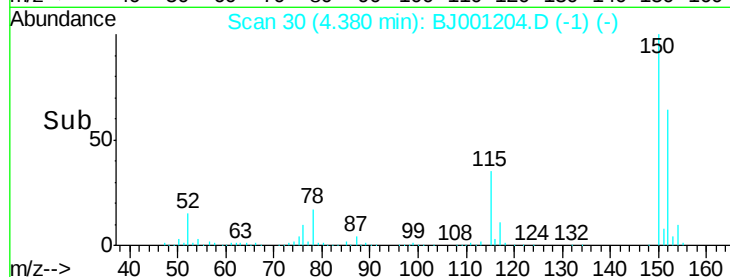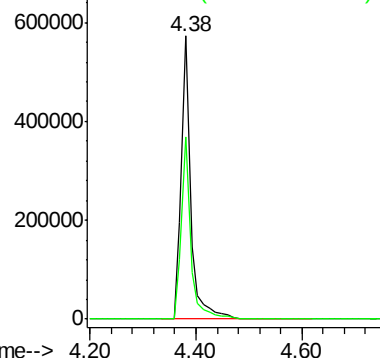



#2

Tripropylphosphate
Concen: 0.00 ug/ml
Expected RT: 6.49 min

Lab File: BJ001204.D
Acq: 12 Nov 2012 15:42

Tgt Ion: 99
Sig Exp Ratio
99 100
141 20.8

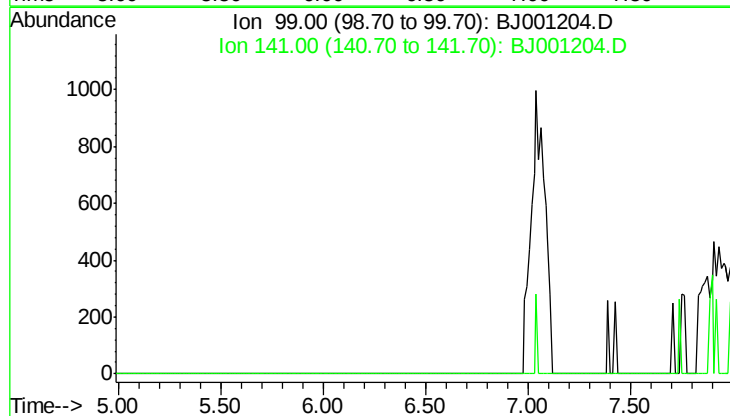

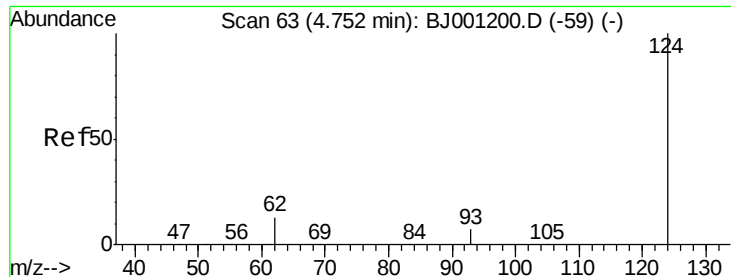

#3

White Phosphorus

Concen: 0.95 ug/ml

RT: 4.75 min Scan# 63

Delta R.T. 0.00 min

Lab File: BJ001204.D

Acq: 12 Nov 2012 15:42

Instrument :

BNA_J

ClientSampleId :

P4-ICV


Tgt Ion:124 Resp: 645521

Ion Ratio Lower Upper

124 100

93 7.4 0.0 27.3

62 15.7 0.0 35.9

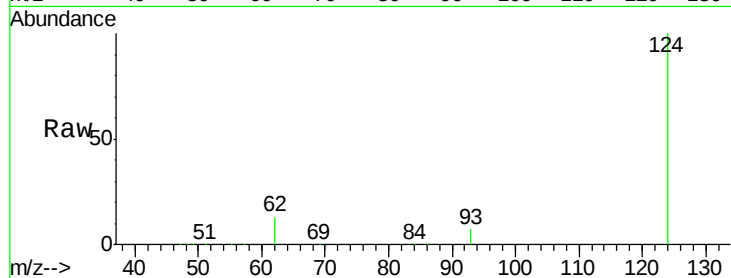

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

