

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001206.D
Acq On : 12 Nov 2012 16:17
Operator : HLM
Sample : PB66741BS
Misc : SOIL BNA_J HLM
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB66741BS

Quant Time: Nov 19 00:20:14 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.39	150	744615	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	6.48	99	1547703	2.58	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	103.20%


Target Compounds					Qvalue
3) White Phosphorus	4.76	124	489793	0.69	ug/ml 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001206.D
Acq On : 12 Nov 2012 16:17
Operator : HLM
Sample : PB66741BS
Misc : SOIL BNA_J HLM
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB66741BS

Quant Time: Nov 19 00:20:14 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

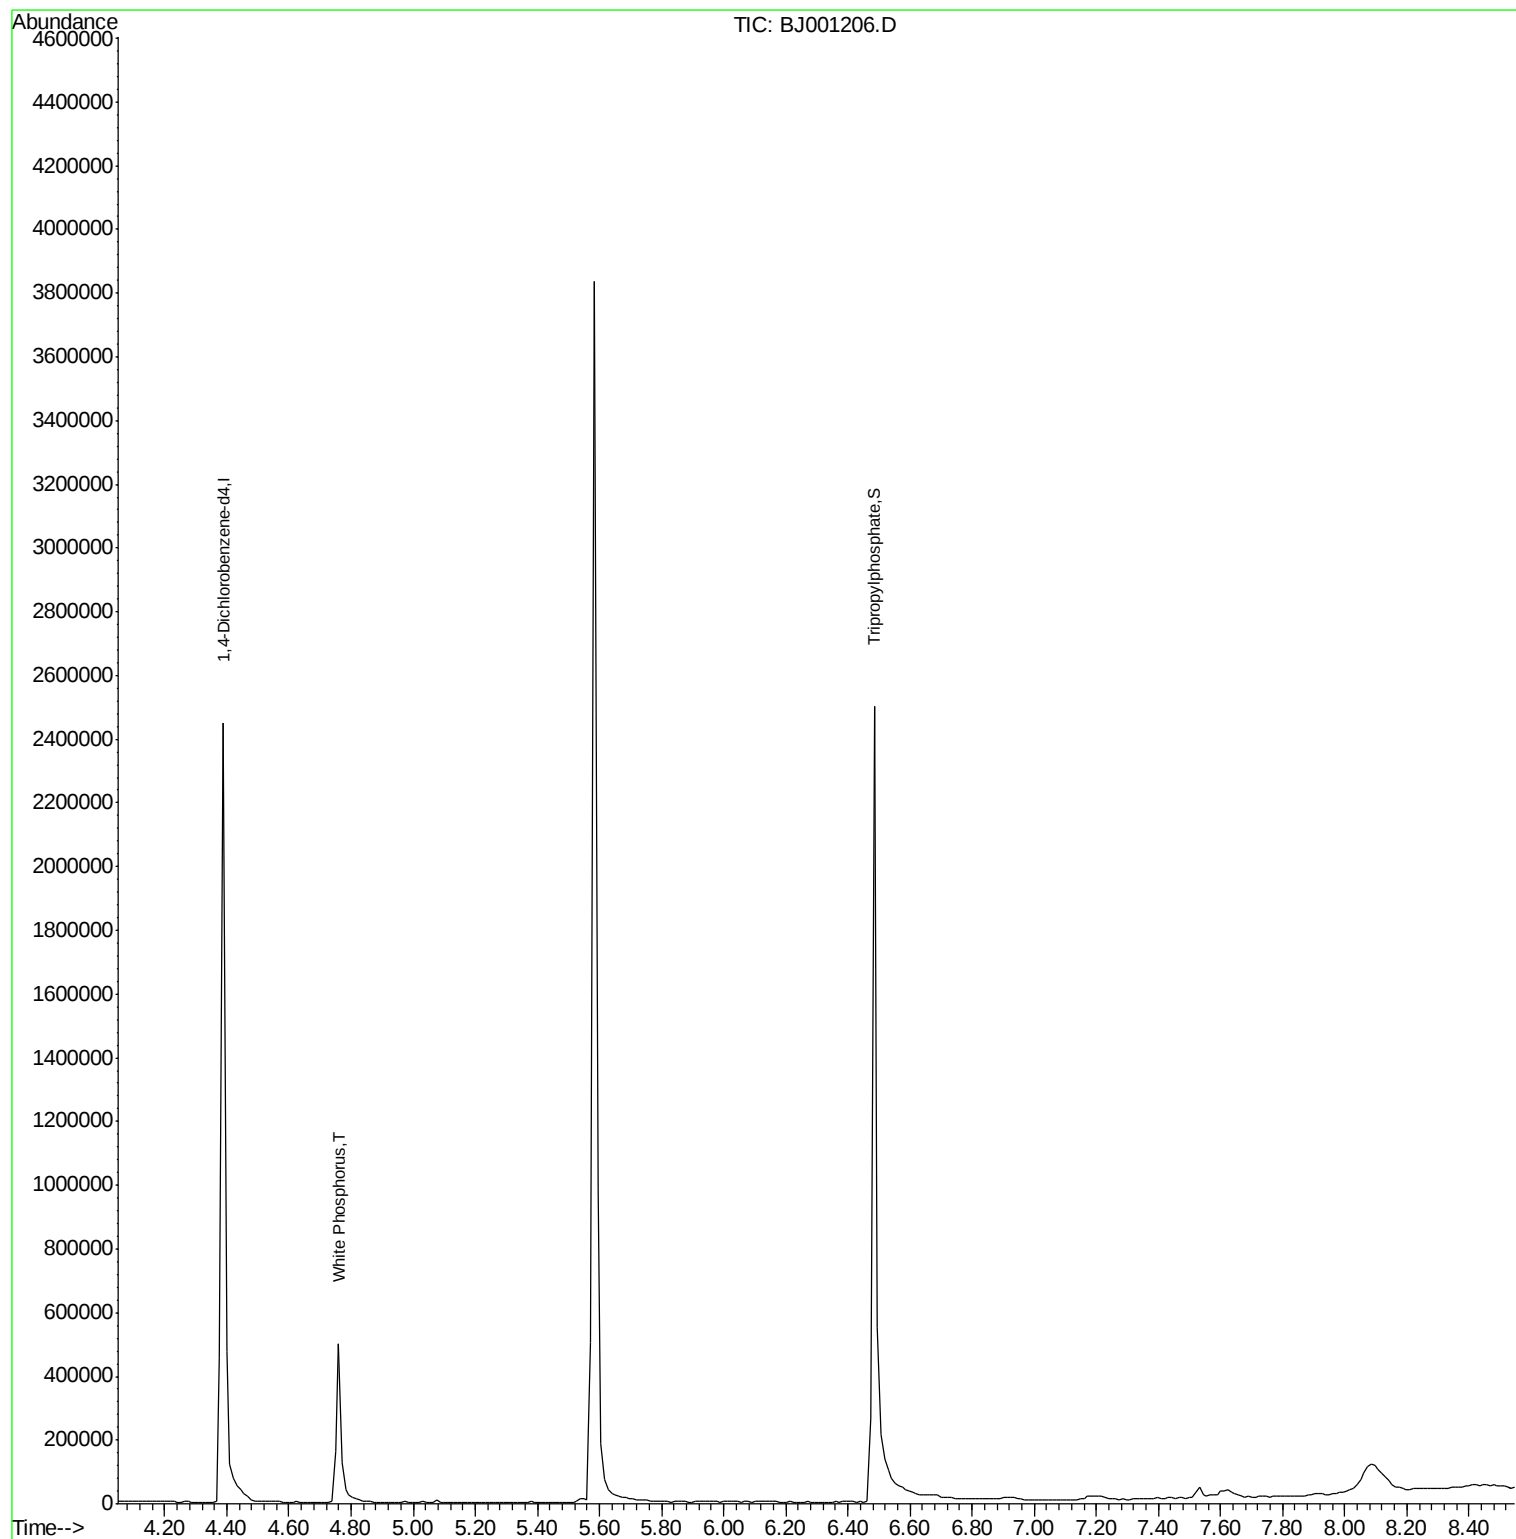

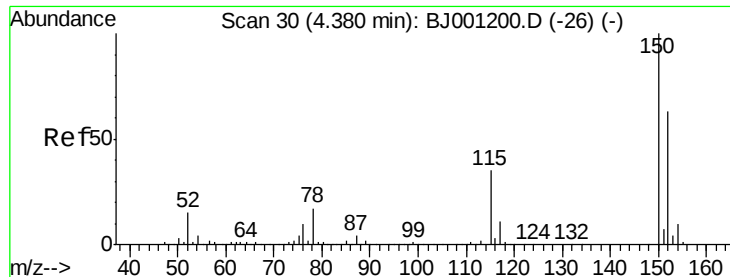


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.39 min Scan# 31
Delta R.T. 0.01 min
Lab File: BJ001206.D
Acq: 12 Nov 2012 16:17

Instrument :
BNA_J
ClientSampleId :
PB66741BS

Tgt Ion:150 Resp: 744615
Ion Ratio Lower Upper
150 100
152 63.5 43.1 83.1

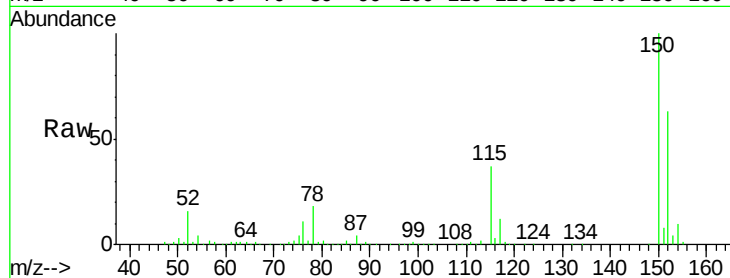


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

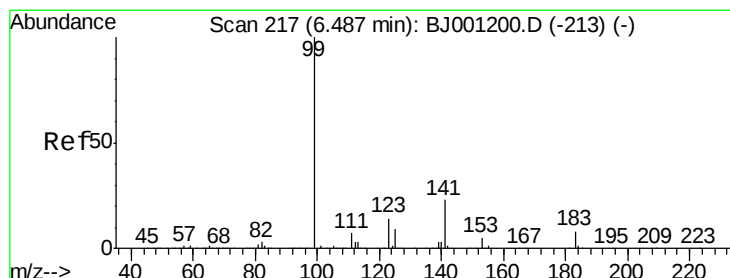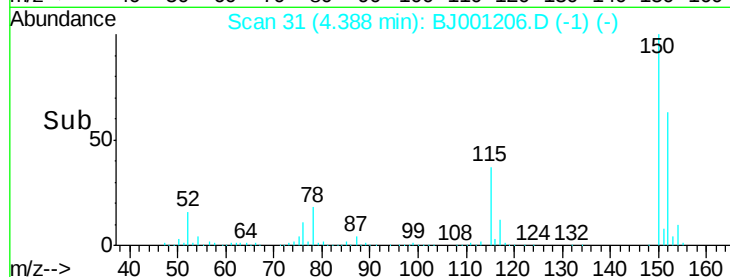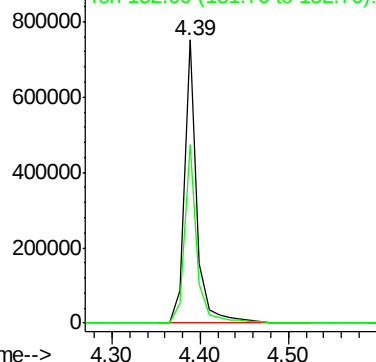



#2


Tripropylphosphate
Concen: 2.58 ug/ml
RT: 6.48 min Scan# 217
Delta R.T. -0.00 min
Lab File: BJ001206.D
Acq: 12 Nov 2012 16:17

Tgt Ion: 99 Resp: 1547703
Ion Ratio Lower Upper
99 100
141 20.3 0.8 40.8

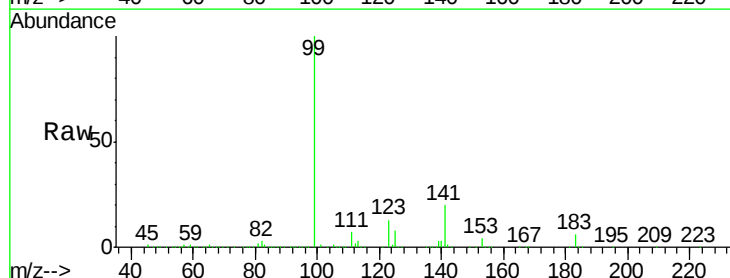

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

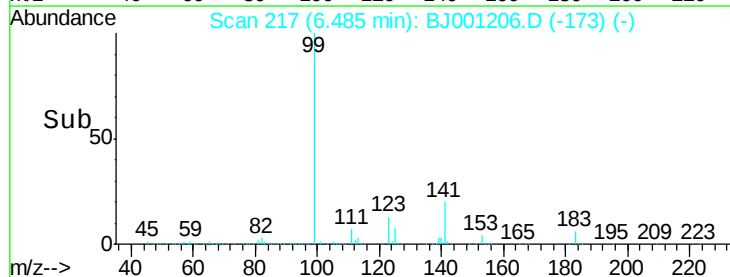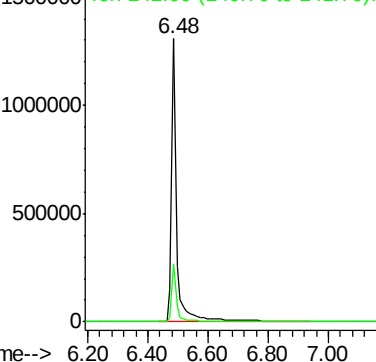

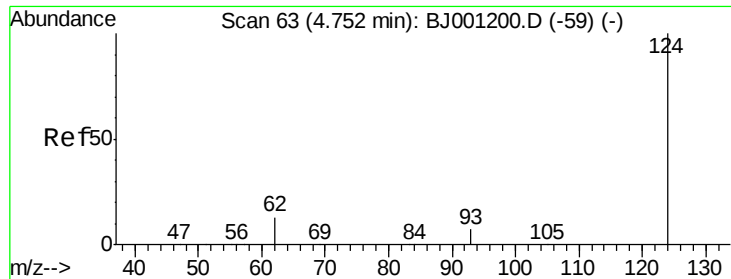

#3
 White Phosphorus
 Concen: 0.69 ug/ml
 RT: 4.76 min Scan# 64
 Delta R.T. 0.01 min
 Lab File: BJ001206.D
 Acq: 12 Nov 2012 16:17

Instrument :
 BNA_J
 ClientSampleId :
 PB66741BS

Tgt Ion:	124	Resp:	489793
Ion	Ratio	Lower	Upper
124	100		
93	7.1	0.0	27.3
62	15.6	0.0	35.9

