

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001207.D
Acq On : 12 Nov 2012 16:30
Operator : HLM
Sample : D4740-01
Misc : SOIL BNA_J HLM
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
REDO-7

Quant Time: Nov 15 16:20:37 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.39	150	743778	2.50	ug/ml	0.01

System Monitoring Compounds

2) Tripropylphosphate	6.50	99	1523198	2.54	ug/ml	0.01
Spiked Amount	2.500	Range	20 - 150	Recovery	=	101.60%


Target Compounds					Qvalue
3) White Phosphorus	4.76	124	96959	0.14	ug/ml 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001207.D
Acq On : 12 Nov 2012 16:30
Operator : HLM
Sample : D4740-01
Misc : SOIL BNA_J HLM
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
REDO-7

Quant Time: Nov 15 16:20:37 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

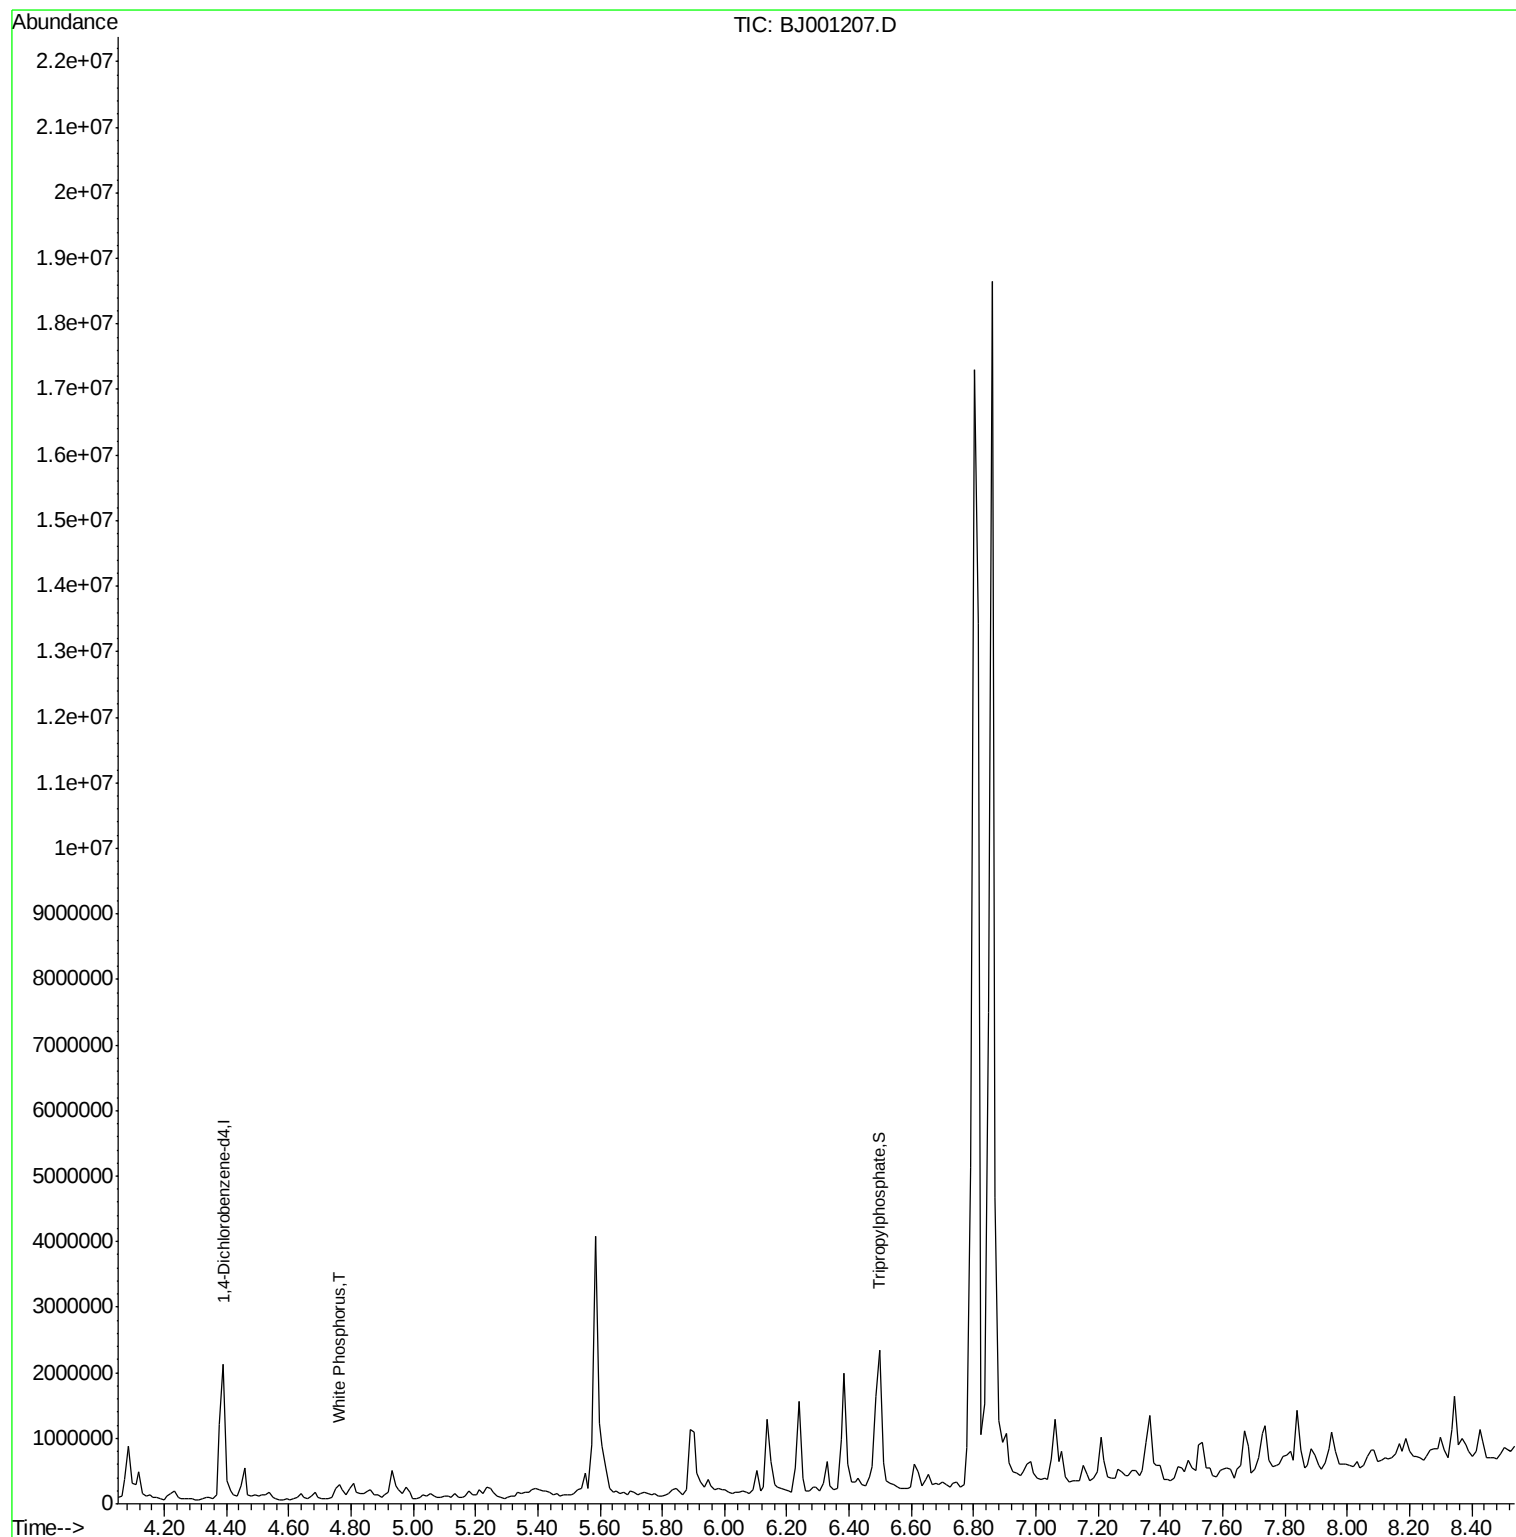




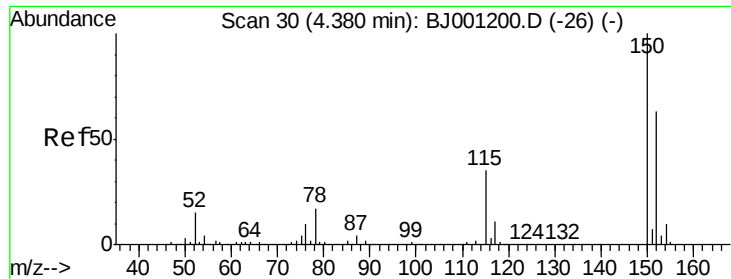


#1

1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.39 min Scan# 31
Delta R.T. 0.01 min
Lab File: BJ001207.D
Acq: 12 Nov 2012 16:30

Instrument :
BNA_J
ClientSampleId :
REDO-7




Tgt Ion:150 Resp: 743778
Ion Ratio Lower Upper
150 100
152 63.4 43.1 83.1

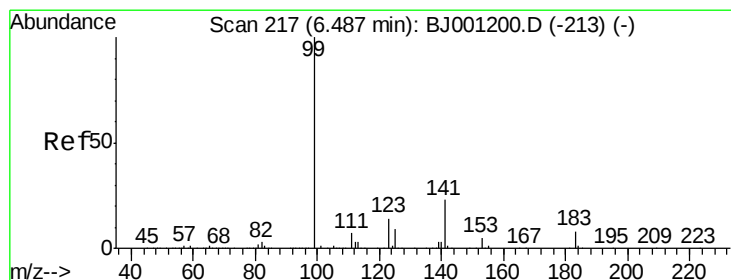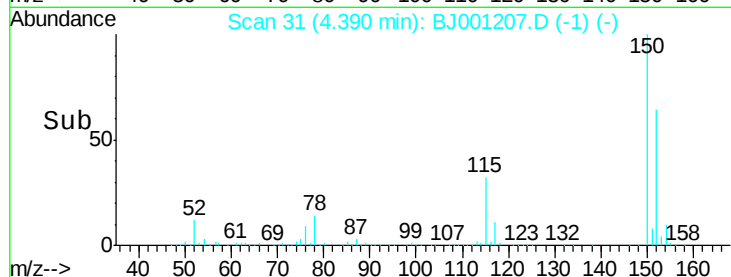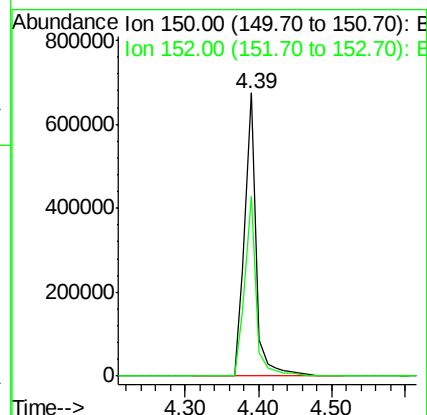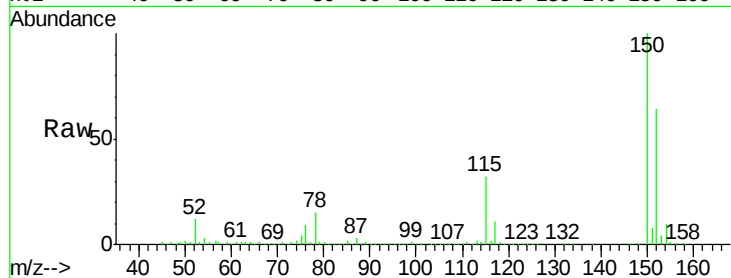


#2

Tripropylphosphate
Concen: 2.54 ug/ml
RT: 6.50 min Scan# 218
Delta R.T. 0.01 min
Lab File: BJ001207.D
Acq: 12 Nov 2012 16:30

Tgt Ion: 99 Resp: 1523198
Ion Ratio Lower Upper
99 100
141 21.5 0.8 40.8

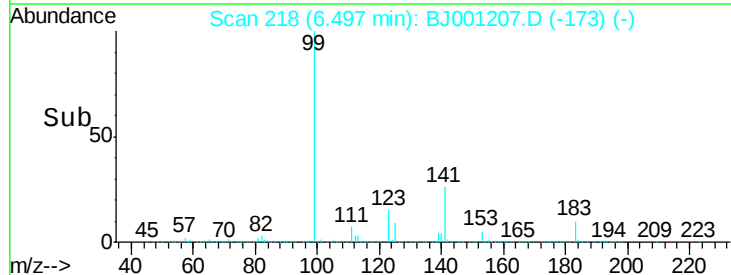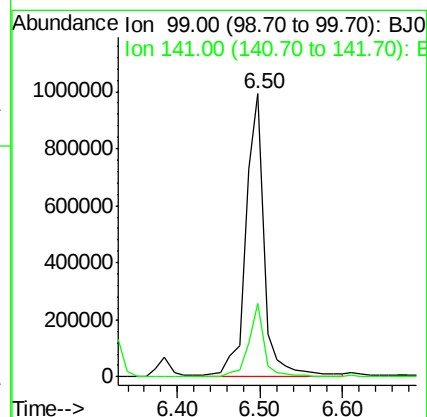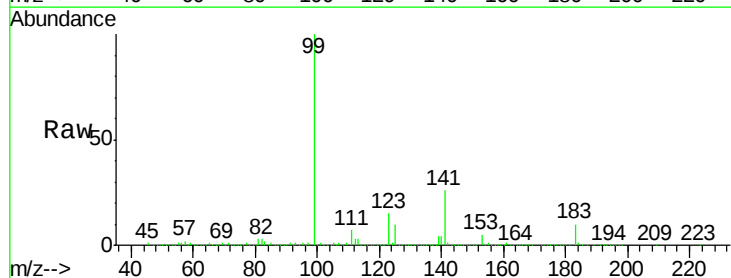

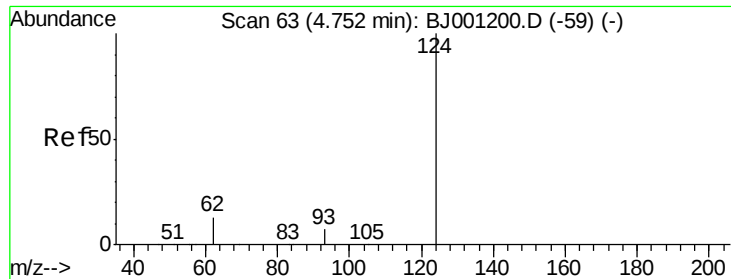

#3
 White Phosphorus
 Concen: 0.14 ug/ml
 RT: 4.76 min Scan# 64
 Delta R.T. 0.01 min
 Lab File: BJ001207.D
 Acq: 12 Nov 2012 16:30

Instrument :
 BNA_J
 ClientSampleId :
 REDO-7

Tgt Ion	Ratio	Lower	Upper
124	100		
93	7.8	0.0	27.3
62	17.4	0.0	35.9

