

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
 Data File : BJ001212.D
 Acq On : 12 Nov 2012 17:36
 Operator : HLM
 Sample : D4740-04
 Misc : SOIL BNA_J HLM
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 REDO-13

Quant Time: Nov 19 00:20:45 2012
 Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
 Quant Title : P4 by SOP M.5
 QLast Update : Mon Nov 12 15:57:53 2012
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.39	150	686187	2.50	ug/ml	0.01

System Monitoring Compounds						
2) Tripropylphosphate	6.52	99	1296793	2.34	ug/ml	0.04
Spiked Amount	2.500	Range	20 - 150	Recovery	=	93.60%


Target Compounds					Qvalue
3) White Phosphorus	4.76	124	136362	0.21	ug/ml 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001212.D
Acq On : 12 Nov 2012 17:36
Operator : HLM
Sample : D4740-04
Misc : SOIL BNA_J HLM
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
REDO-13

Quant Time: Nov 19 00:20:45 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

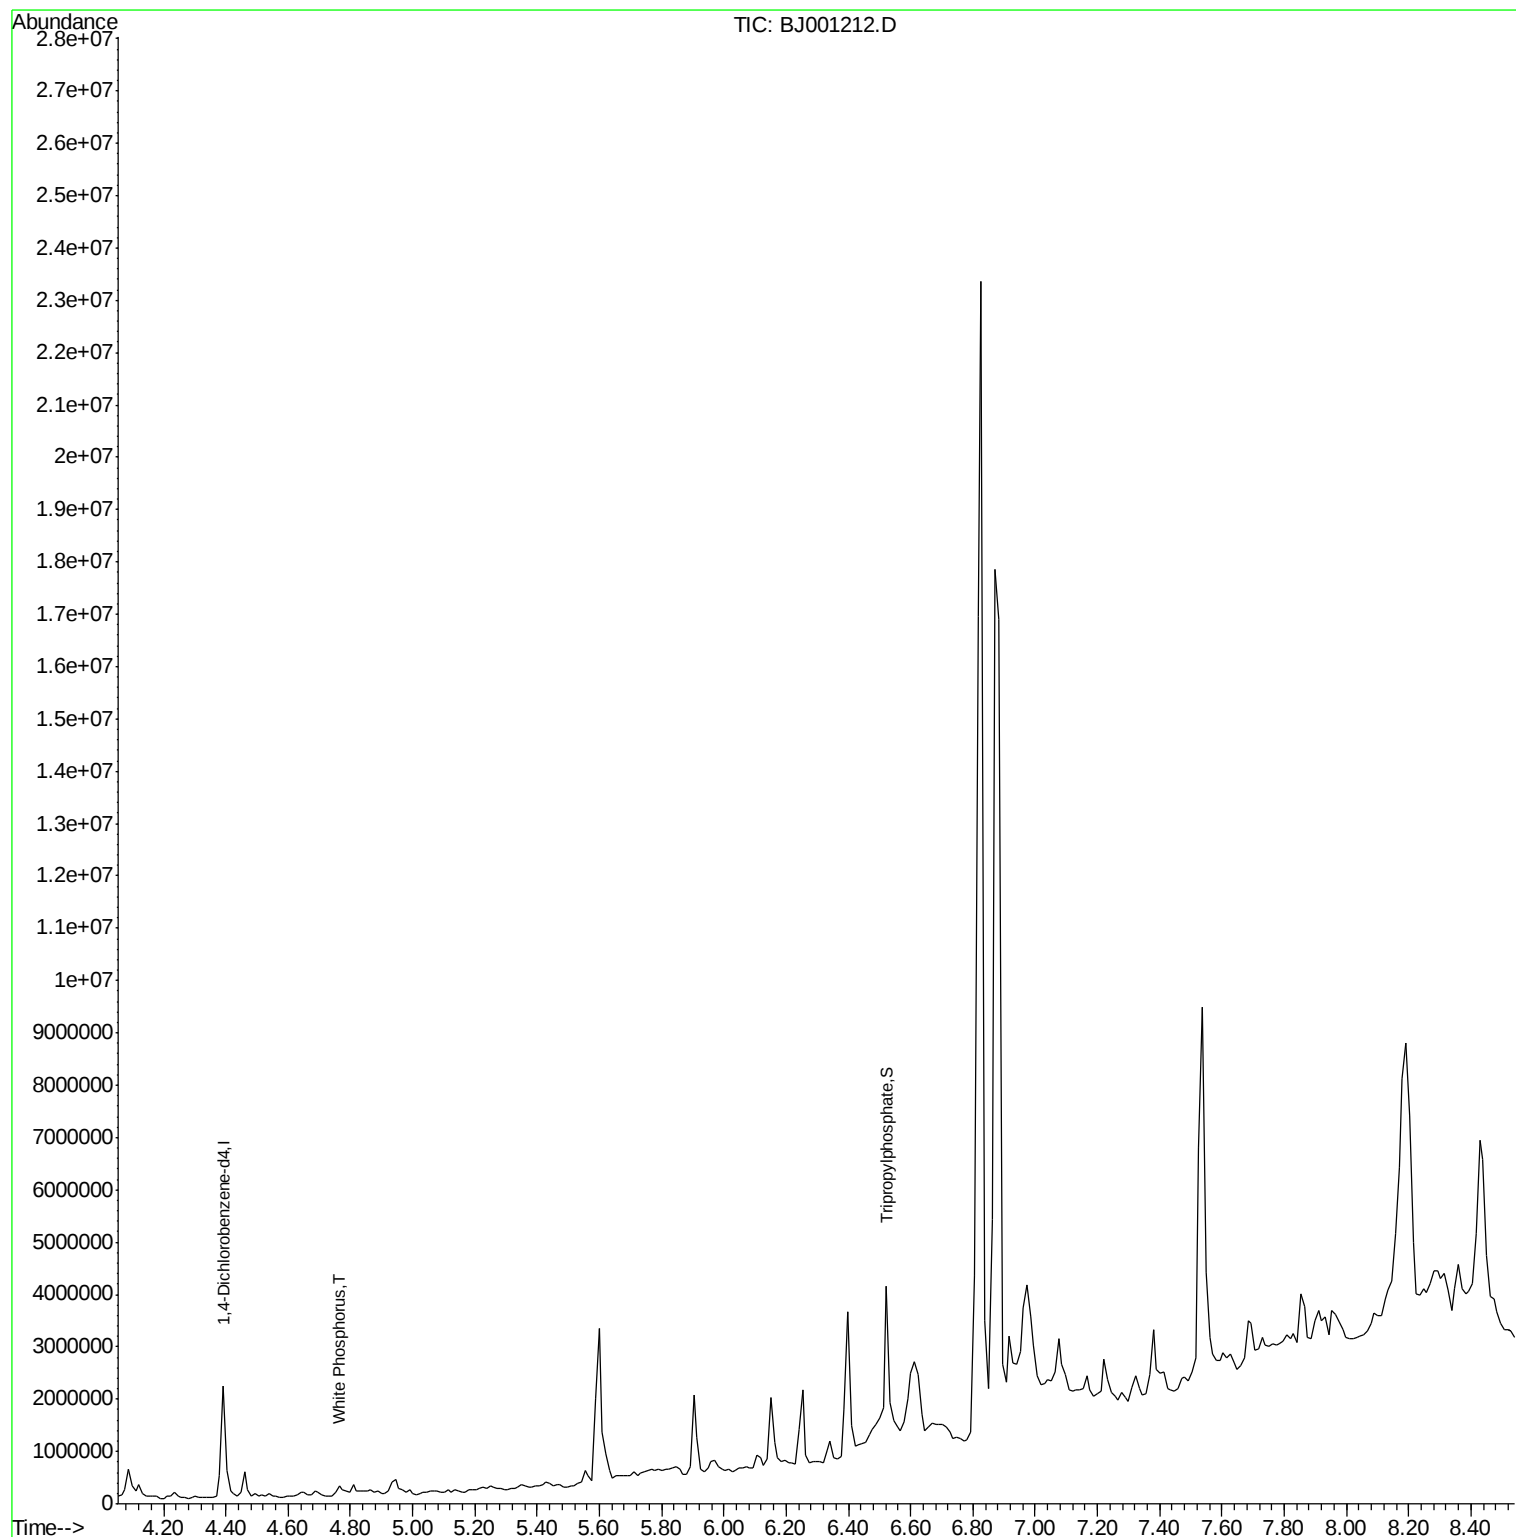

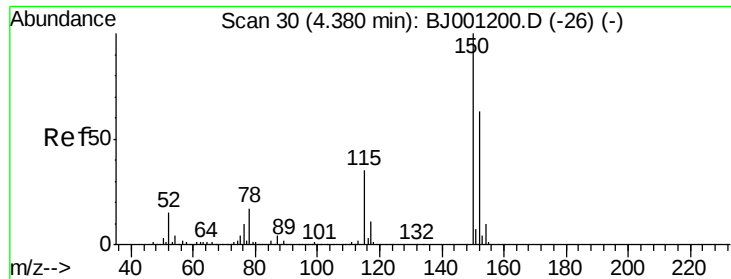


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.39 min Scan# 31
Delta R.T. 0.01 min
Lab File: BJ001212.D
Acq: 12 Nov 2012 17:36

Instrument :
BNA_J
ClientSampleId :
REDO-13

Tgt Ion:150 Resp: 686187
Ion Ratio Lower Upper
150 100
152 63.4 43.1 83.1

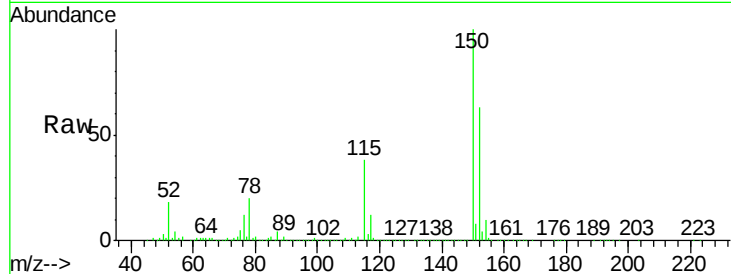


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

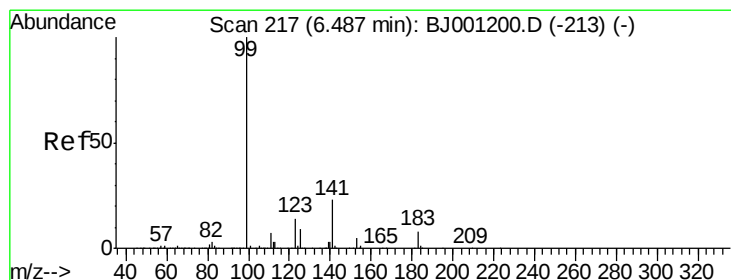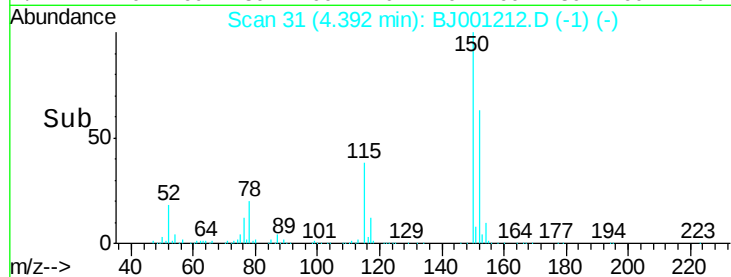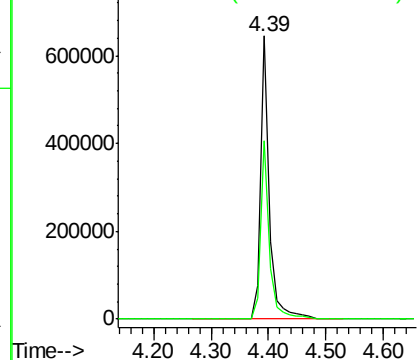



#2


Trippropylphosphate
Concen: 2.34 ug/ml
RT: 6.52 min Scan# 220
Delta R.T. 0.04 min
Lab File: BJ001212.D
Acq: 12 Nov 2012 17:36

Tgt Ion: 99 Resp: 1296793
Ion Ratio Lower Upper
99 100
141 21.7 0.8 40.8

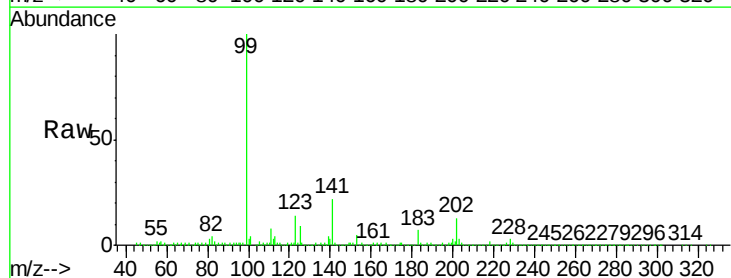

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

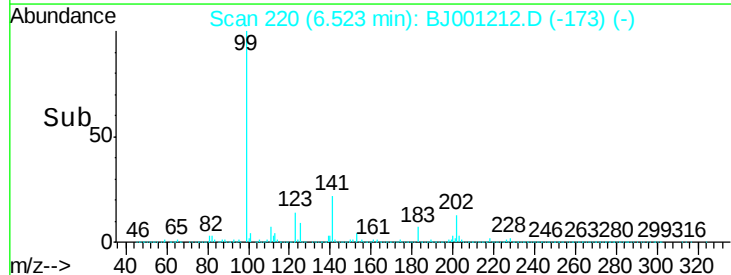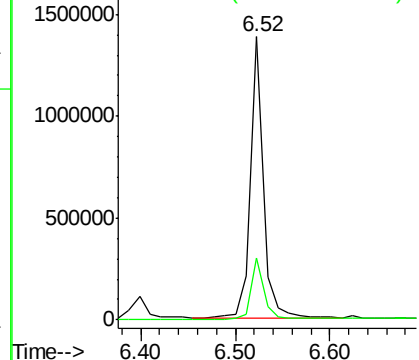

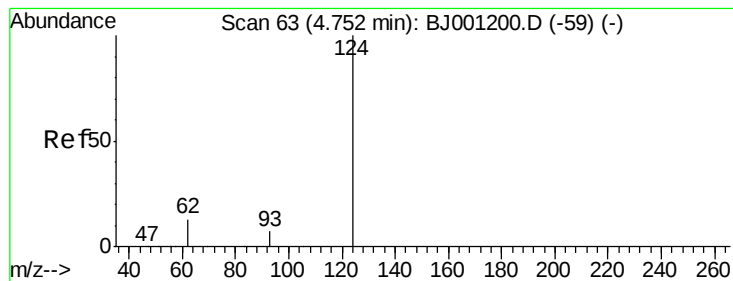

#3

White Phosphorus

Concen: 0.21 ug/ml

RT: 4.76 min Scan# 64

Delta R.T. 0.01 min

Lab File: BJ001212.D

Acq: 12 Nov 2012 17:36

Instrument :

BNA_J

ClientSampleId :

REDO-13


Tgt Ion:124 Resp: 136362

Ion Ratio Lower Upper

124 100

93 8.4 0.0 27.3

62 19.6 0.0 35.9

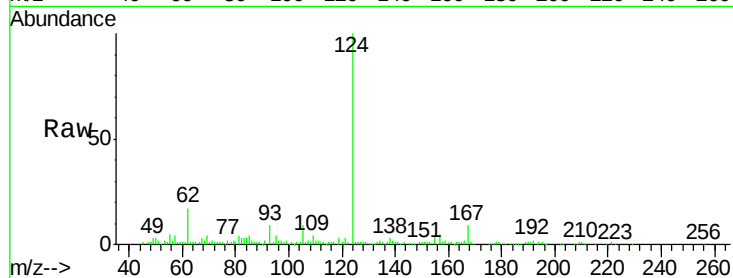

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

