

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001214.D
Acq On : 12 Nov 2012 18:02
Operator : HLM
Sample : D4740-06
Misc : SOIL BNA_J HLM
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
REDO-15

Quant Time: Nov 19 00:20:51 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.39	150	682809	2.50	ug/ml	0.01

System Monitoring Compounds

2) Tripropylphosphate	6.53	99	1181278	2.15	ug/ml	0.05
Spiked Amount	2.500	Range	20 - 150	Recovery	=	86.00%


Target Compounds					Qvalue
3) White Phosphorus	4.78	124	103626	0.16	ug/ml 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001214.D
Acq On : 12 Nov 2012 18:02
Operator : HLM
Sample : D4740-06
Misc : SOIL BNA_J HLM
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
REDO-15

Quant Time: Nov 19 00:20:51 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

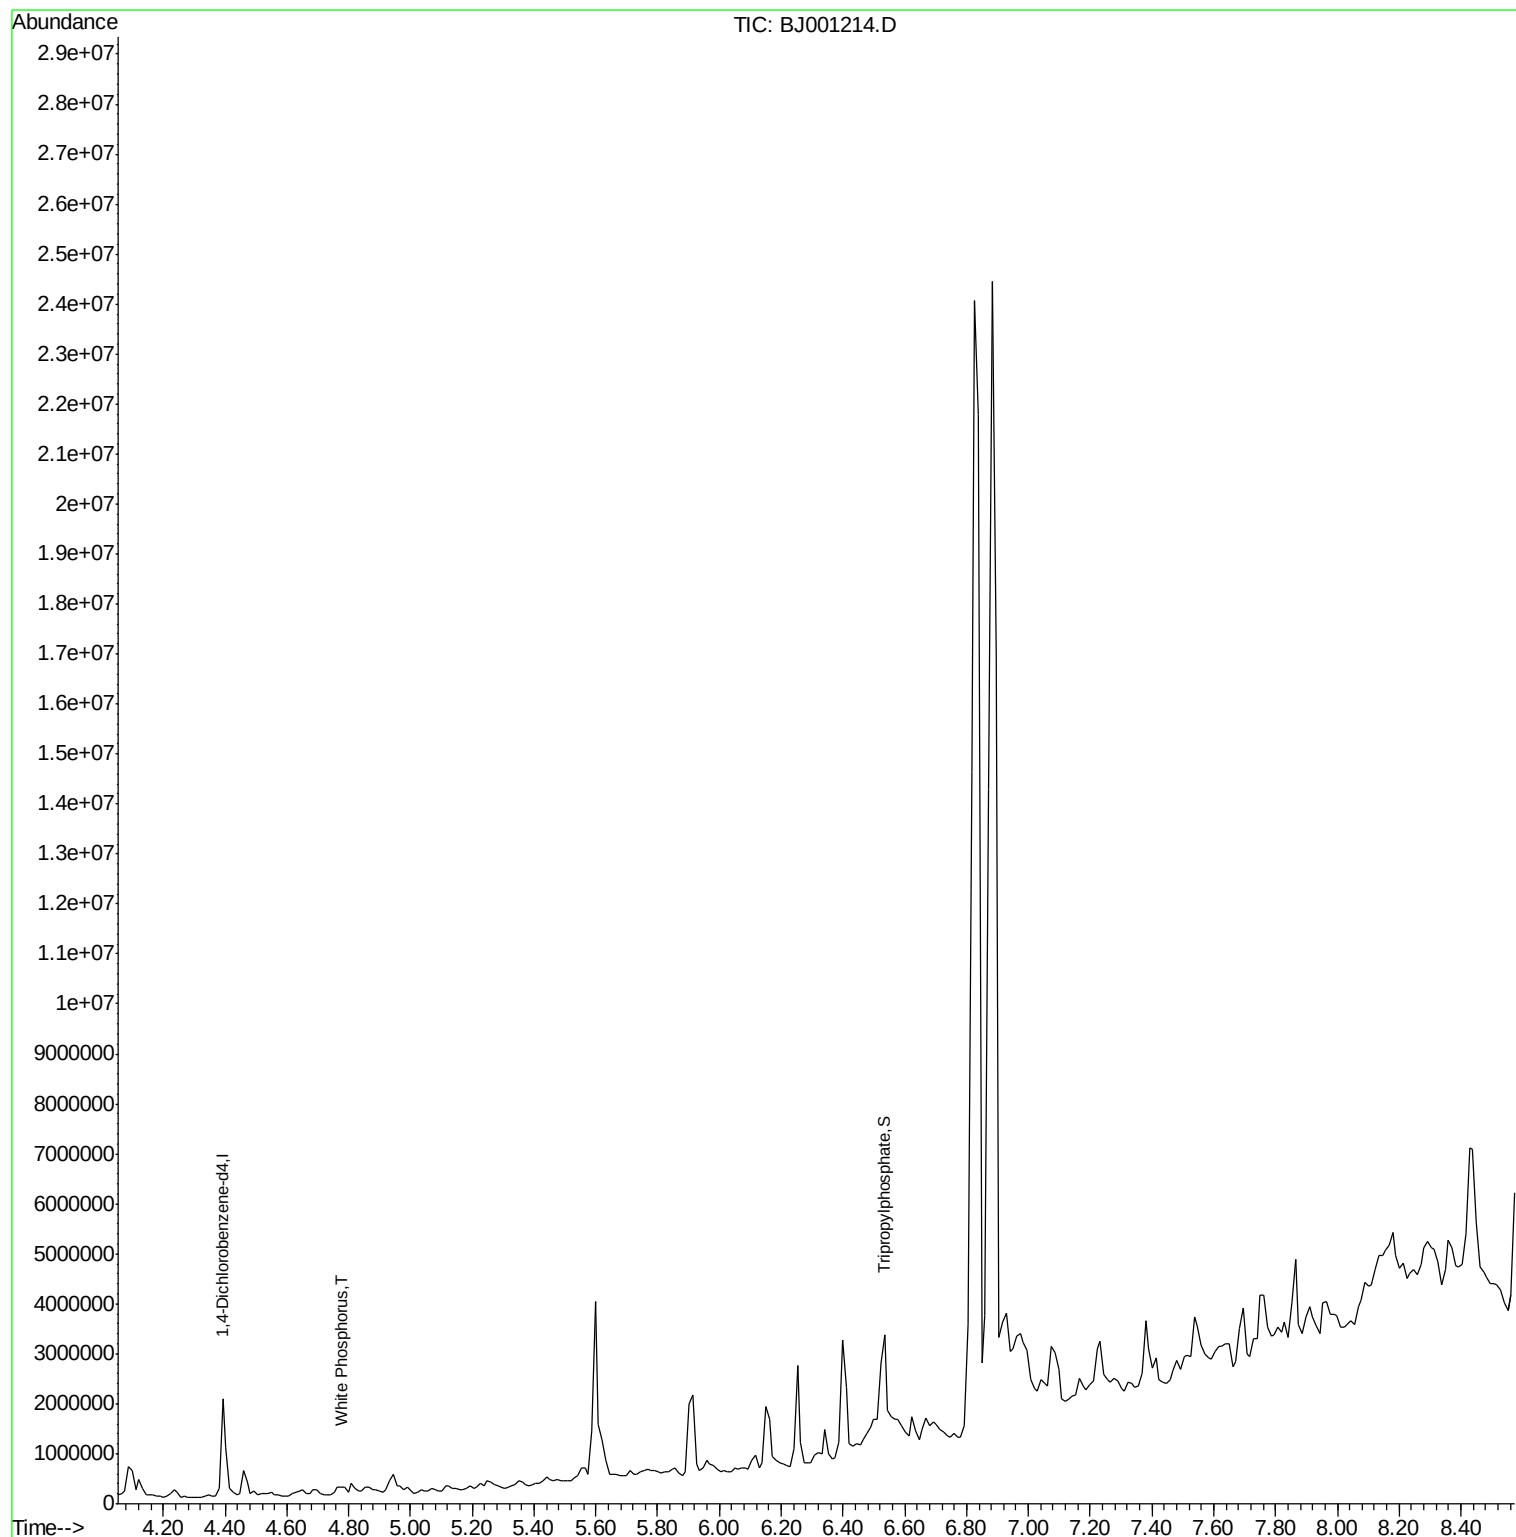

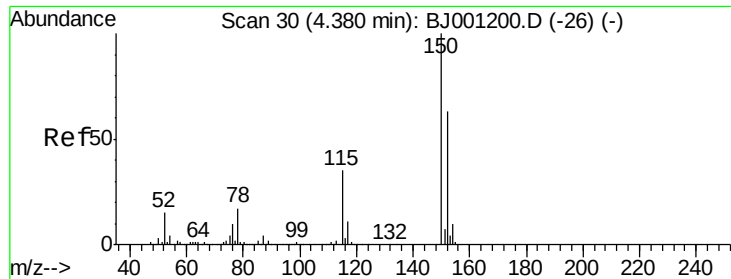


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.39 min Scan# 31
Delta R.T. 0.01 min
Lab File: BJ001214.D
Acq: 12 Nov 2012 18:02

Instrument :
BNA_J
ClientSampled :
REDO-15

Tgt Ion:150 Resp: 682809
Ion Ratio Lower Upper
150 100
152 63.4 43.1 83.1

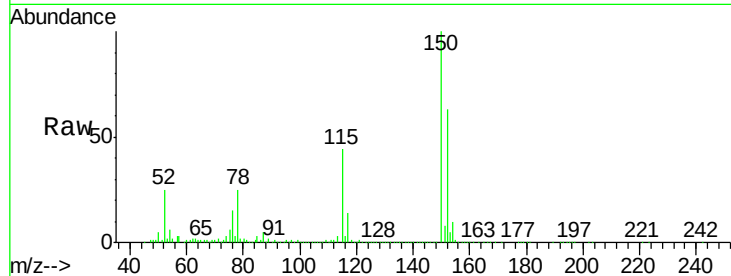


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

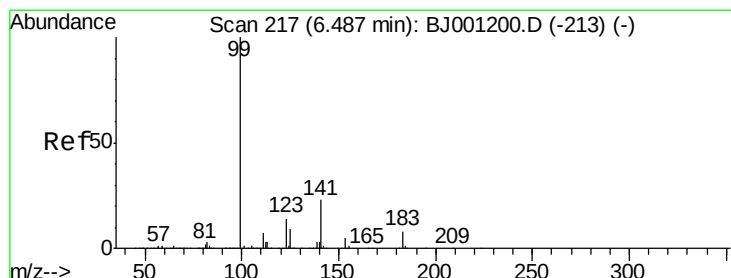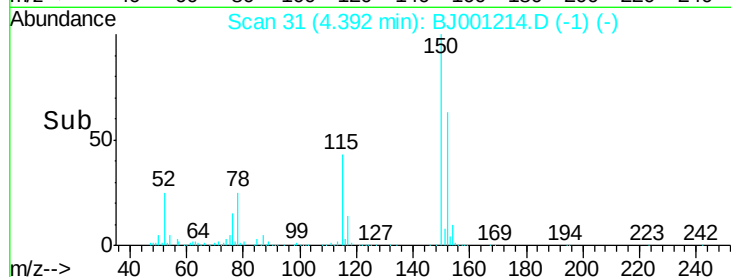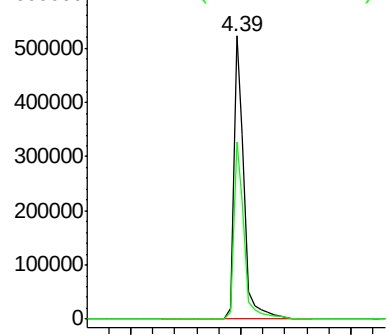



#2


Tripropylphosphate
Concen: 2.15 ug/ml
RT: 6.53 min Scan# 221
Delta R.T. 0.05 min
Lab File: BJ001214.D
Acq: 12 Nov 2012 18:02

Tgt Ion: 99 Resp: 1181278
Ion Ratio Lower Upper
99 100
141 22.3 0.8 40.8

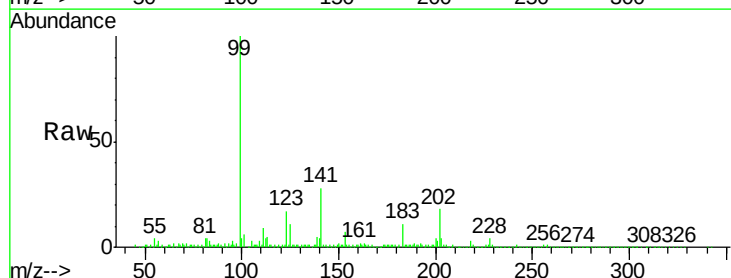

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

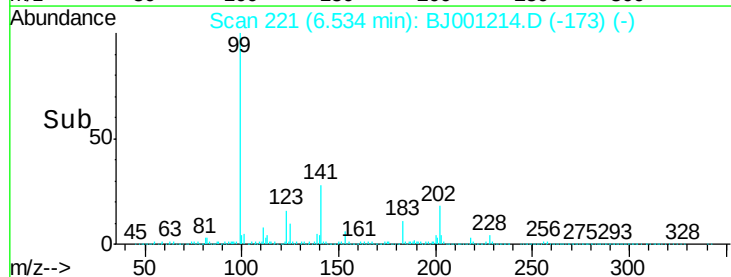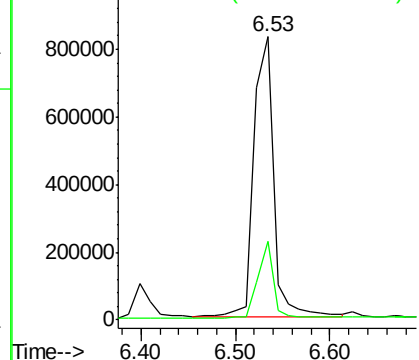

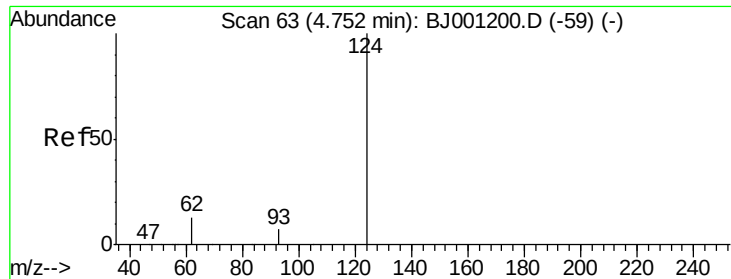

#3
 White Phosphorus
 Concen: 0.16 ug/ml
 RT: 4.78 min Scan# 65
 Delta R.T. 0.02 min
 Lab File: BJ001214.D
 Acq: 12 Nov 2012 18:02

Instrument :
 BNA_J
 ClientSampleId :
 REDO-15

Tgt Ion:	124	Resp:	103626
Ion	Ratio	Lower	Upper
124	100		
93	7.8	0.0	27.3
62	22.0	0.0	35.9

