

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001219.D
Acq On : 12 Nov 2012 19:08
Operator : HLM
Sample : PB66268BL
Misc : WATER BNA_J HLM
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB66268BL

Quant Time: Nov 15 18:25:31 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.40	150	698849	2.50	ug/ml	0.02

System Monitoring Compounds

2) Tripropylphosphate	6.52	99	1288338	2.29	ug/ml	0.03
Spiked Amount	2.500	Range	20 - 150	Recovery	=	91.60%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001219.D
Acq On : 12 Nov 2012 19:08
Operator : HLM
Sample : PB66268BL
Misc : WATER BNA_J HLM
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB66268BL

Quant Time: Nov 15 18:25:31 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

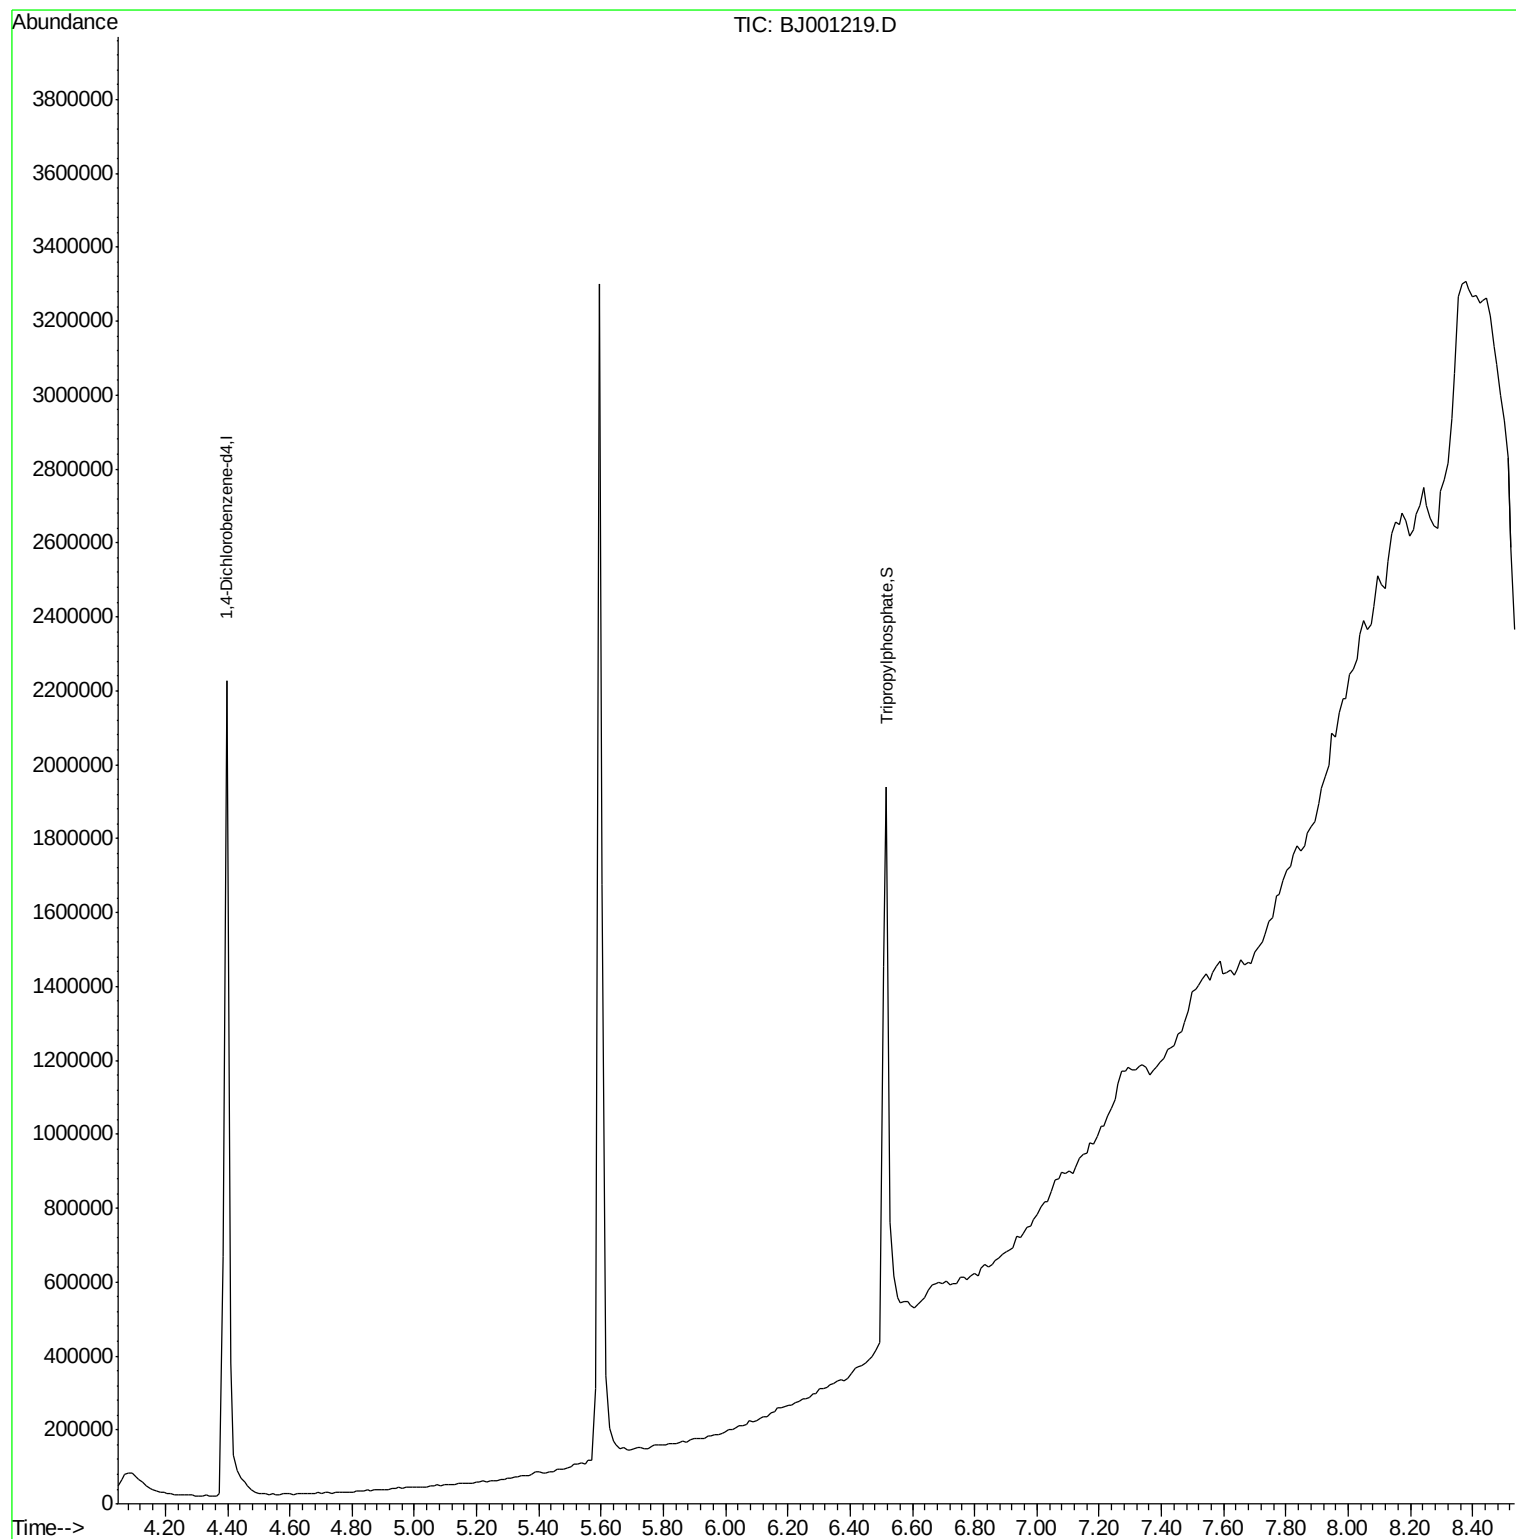

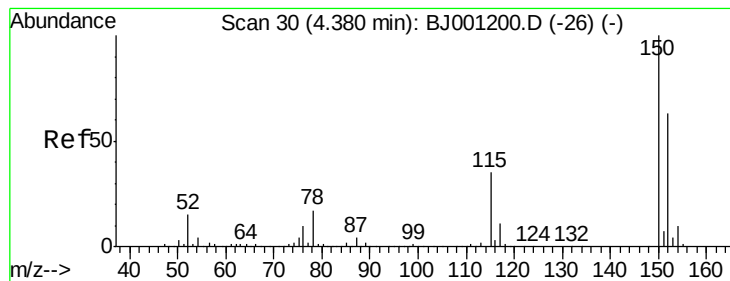


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.40 min Scan# 32
Delta R.T. 0.02 min
Lab File: BJ001219.D
Acq: 12 Nov 2012 19:08

Instrument :
BNA_J
ClientSampleId :
PB66268BL

Tgt Ion:150 Resp: 698849
Ion Ratio Lower Upper
150 100
152 64.0 43.1 83.1

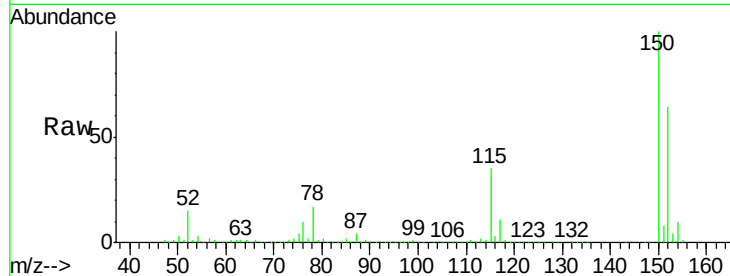


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

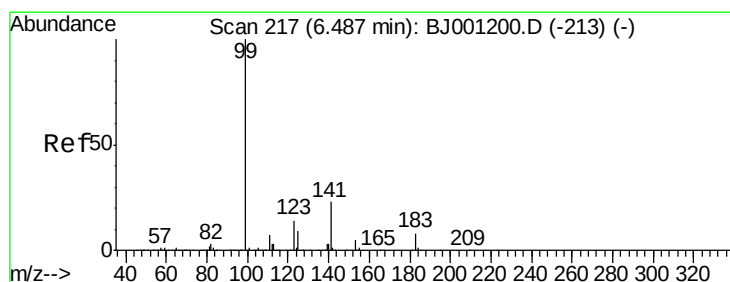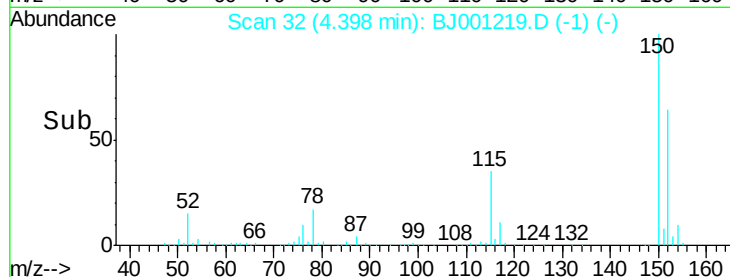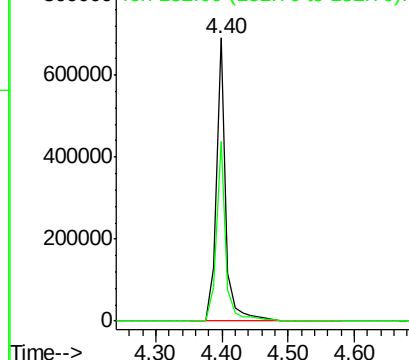

#2

Tripropylphosphate
Concen: 2.29 ug/ml
RT: 6.52 min Scan# 220
Delta R.T. 0.03 min
Lab File: BJ001219.D
Acq: 12 Nov 2012 19:08

Tgt Ion: 99 Resp: 1288338
Ion Ratio Lower Upper
99 100
141 21.3 0.8 40.8

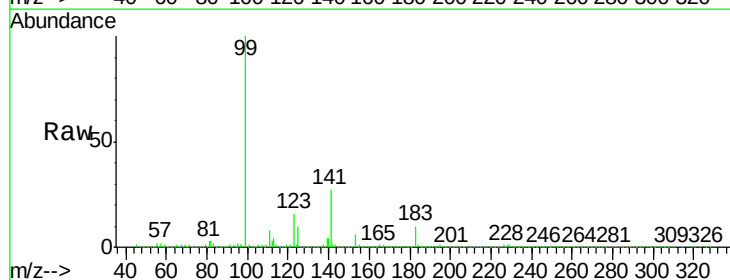

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

