

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001222.D
Acq On : 12 Nov 2012 19:48
Operator : HLM
Sample : D4468-04
Misc : WATER LOQ BNA_J HLM
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
LOQ Water 2012-04

Quant Time: Nov 19 00:21:26 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.40	150	675309	2.50	ug/ml	0.02

System Monitoring Compounds

2) Tripropylphosphate	6.51	99	1417860	2.60	ug/ml	0.02
Spiked Amount	2.500	Range	20 - 150	Recovery	=	104.00%


Target Compounds					Qvalue
3) White Phosphorus	4.77	124	91860	0.14	ug/ml 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ111212\
Data File : BJ001222.D
Acq On : 12 Nov 2012 19:48
Operator : HLM
Sample : D4468-04
Misc : WATER LOQ BNA_J HLM
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
LOQ Water 2012-04

Quant Time: Nov 19 00:21:26 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 12 15:57:53 2012
Response via : Initial Calibration

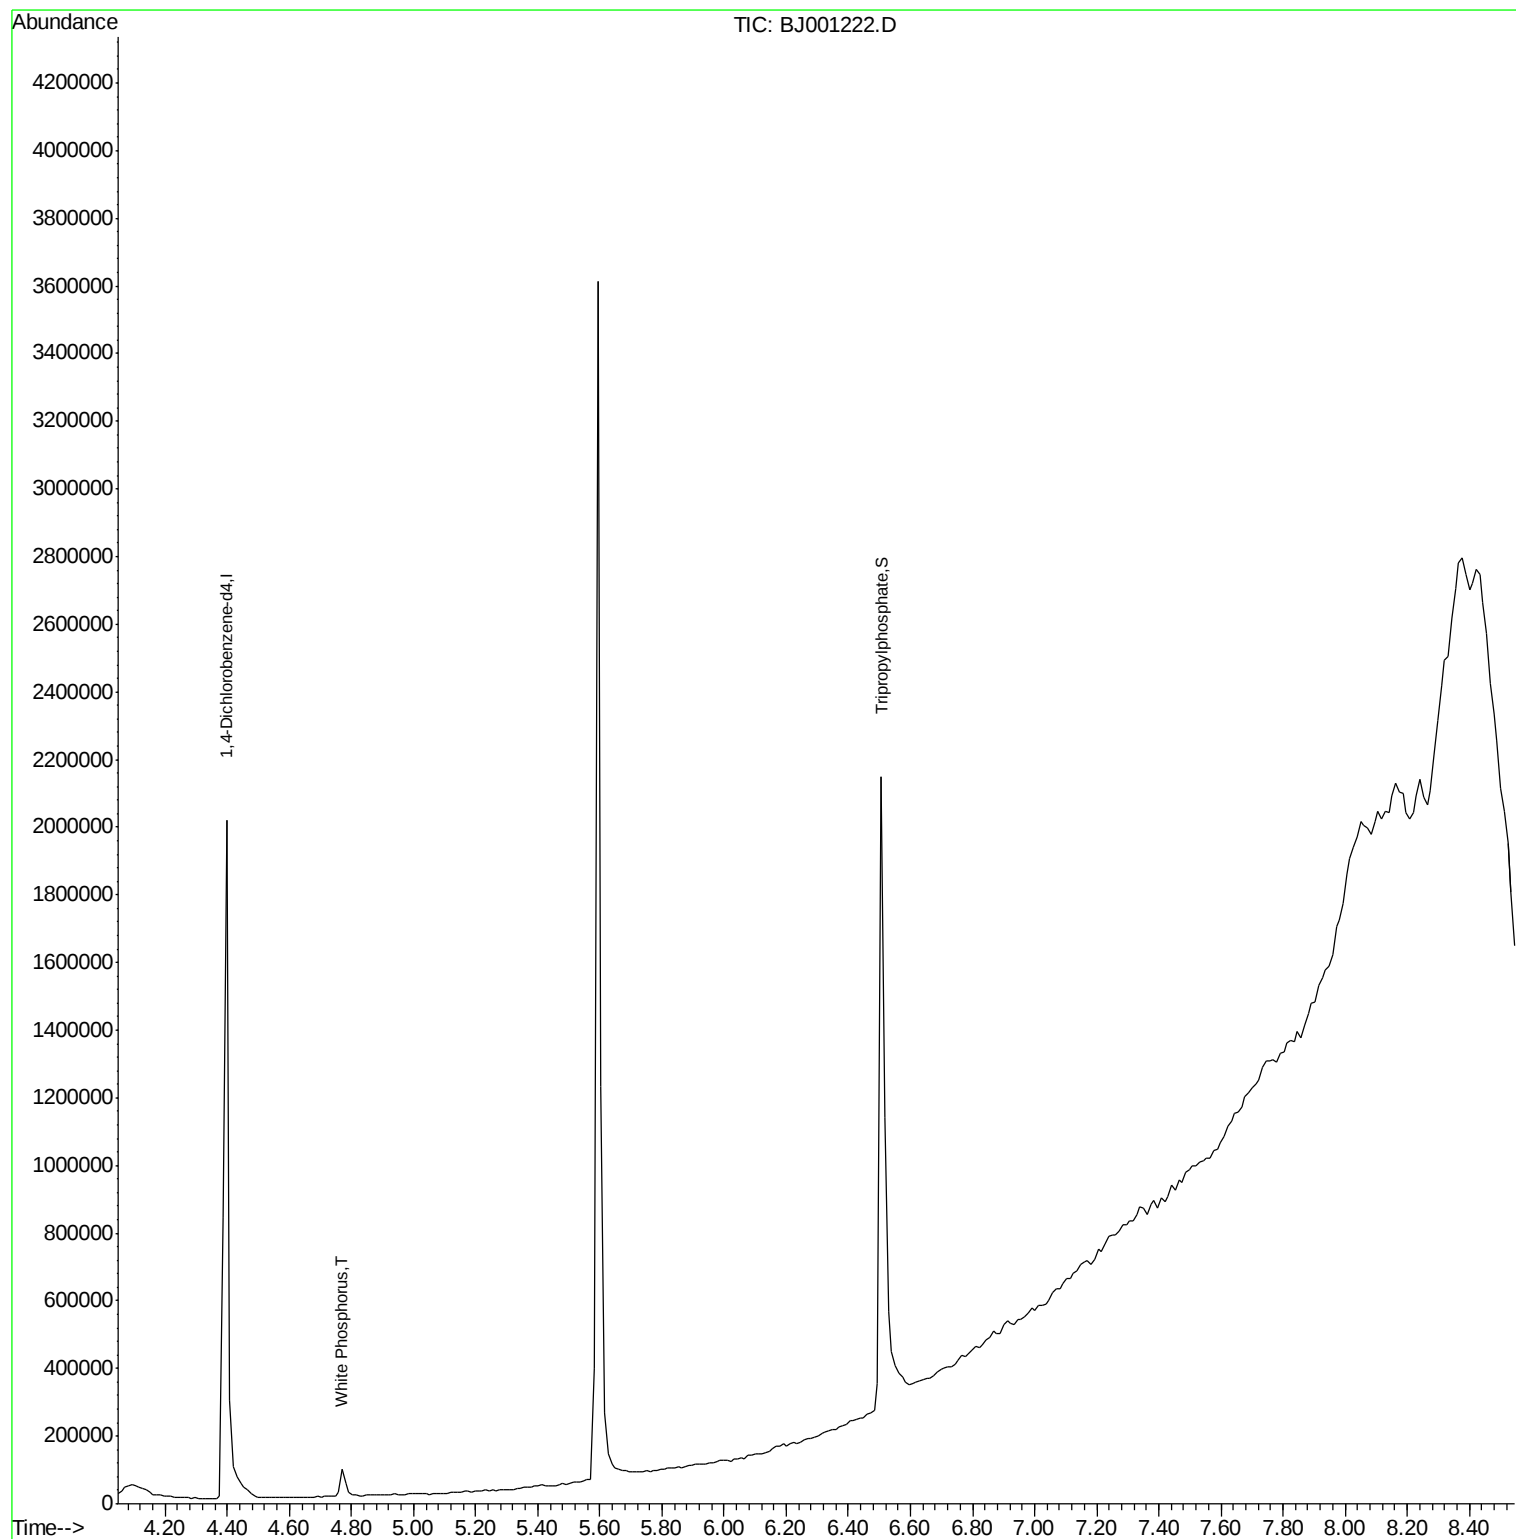

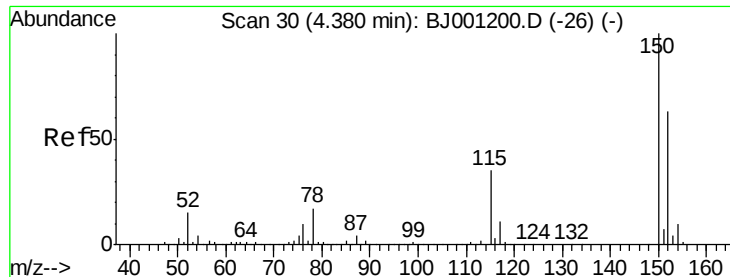


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.40 min Scan# 32
Delta R.T. 0.02 min
Lab File: BJ001222.D
Acq: 12 Nov 2012 19:48

Instrument :
BNA_J
ClientSampleId :
LOQ Water 2012-04

Tgt Ion:150 Resp: 675309
Ion Ratio Lower Upper
150 100
152 63.8 43.1 83.1

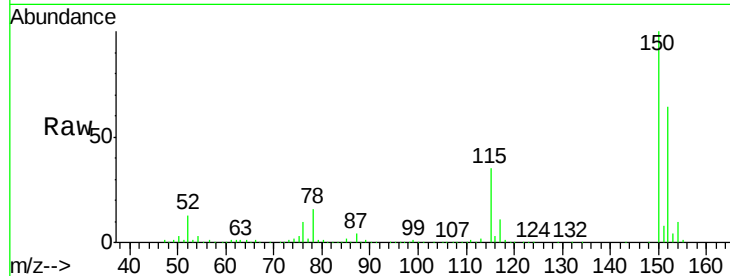


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

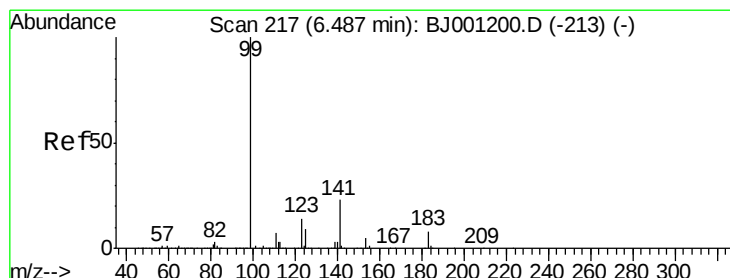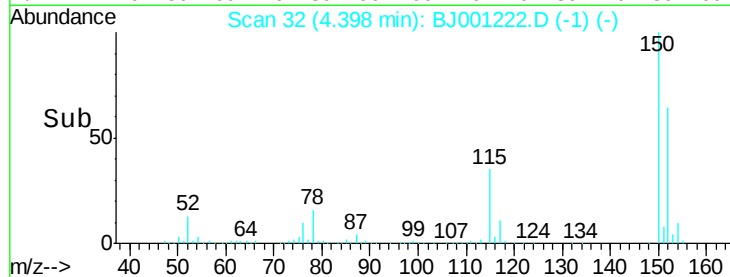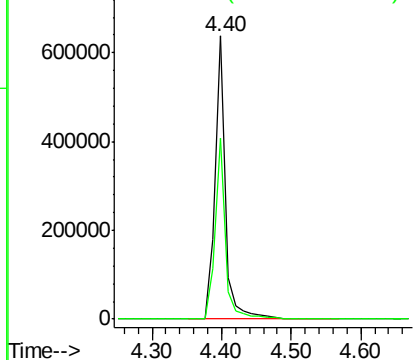



#2


Tripropylphosphate
Concen: 2.60 ug/ml
RT: 6.51 min Scan# 219
Delta R.T. 0.02 min
Lab File: BJ001222.D
Acq: 12 Nov 2012 19:48

Tgt Ion: 99 Resp: 1417860
Ion Ratio Lower Upper
99 100
141 20.4 0.8 40.8

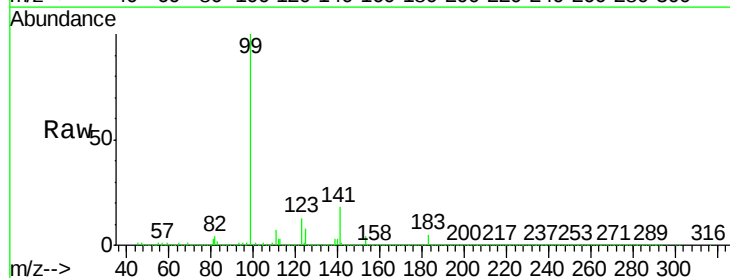

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

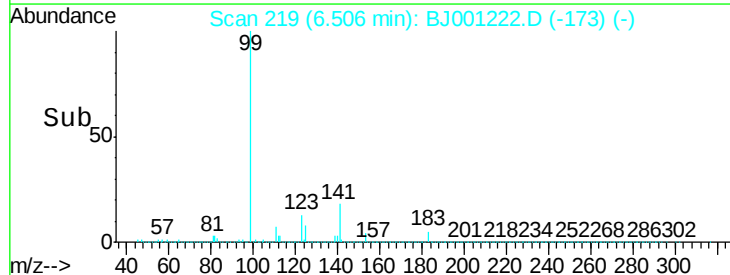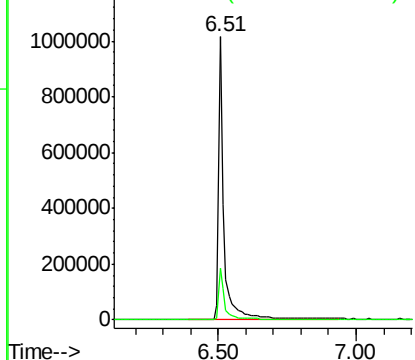

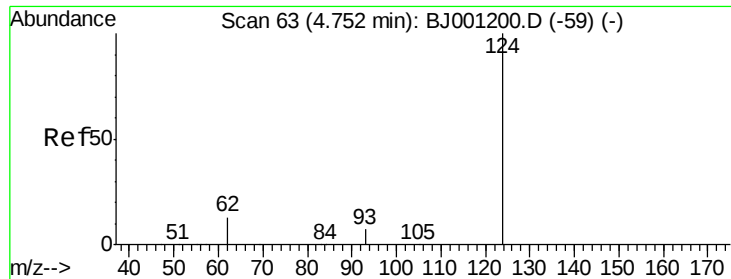

#3

White Phosphorus

Concen: 0.14 ug/ml

RT: 4.77 min Scan# 65

Delta R.T. 0.02 min

Lab File: BJ001222.D


Acq: 12 Nov 2012 19:48

Instrument :

BNA_J

ClientSampleId :

LOQ Water 2012-04

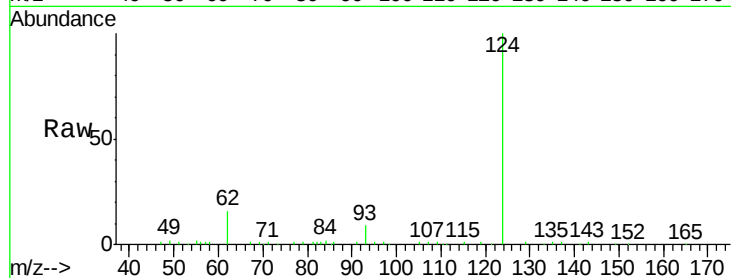


Tgt Ion:124 Resp: 91860

Ion Ratio Lower Upper

124 100

93 7.4 0.0 27.3

62 15.4 0.0 35.9

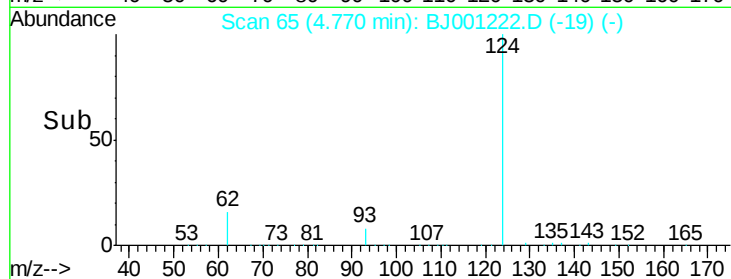

Abundance Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

