

DFTPP

Data File : H:\VOL1\GCMSDATA\J\121112\BJ001196.D

Vial: 1

Acq On : 12 Nov 2012 13:52

Operator: HLM

Sample : DFTPP050

Inst : BNA_J

Misc : DFTPP050 BNA_J HLM

Multiplr: 1.00

MS Integration Params: RTEINT.P

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)



Title : P4 by SOP M.5

Instrument :

BNA_J

ClientSampleId :

DFTPP050

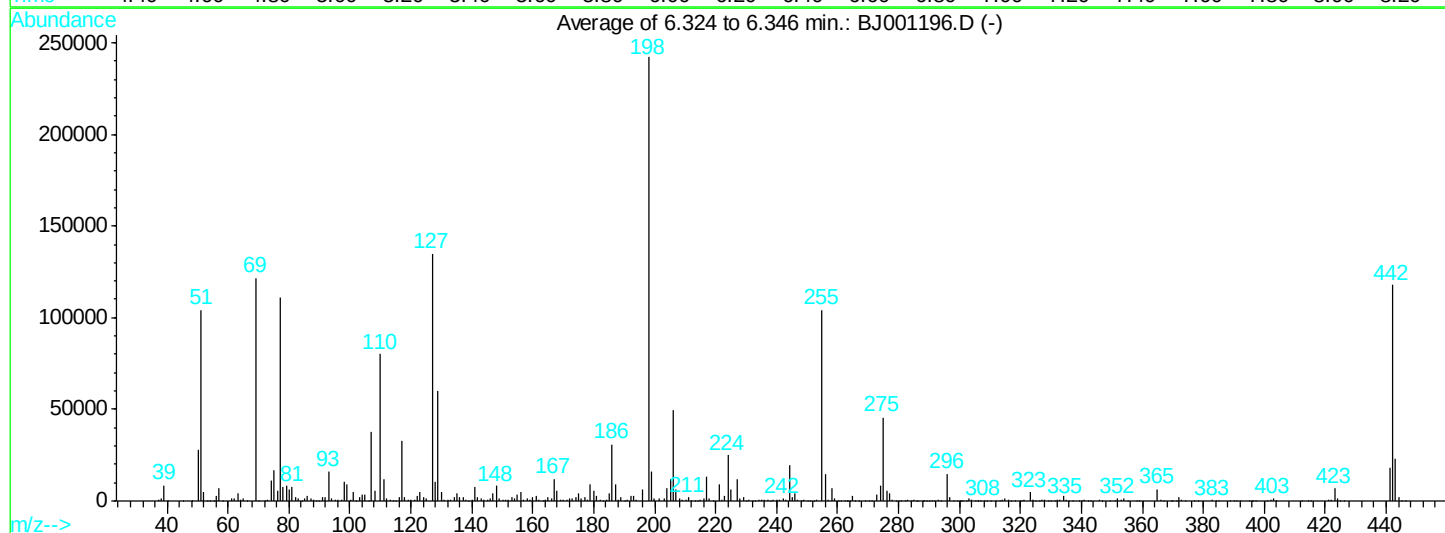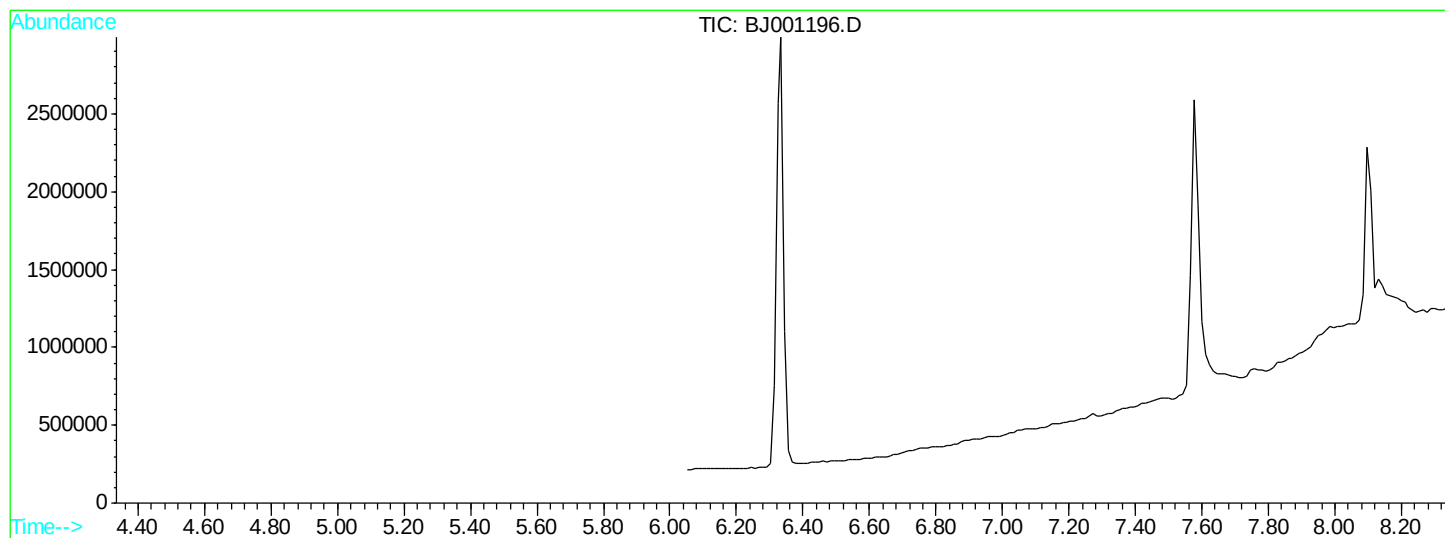

AutoFind: Scans 25, 26, 27; Background Corrected with Scan 14

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	30	60	43.1	104328	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.3	121841	PASS
70	69	0.00	2	0.3	331	PASS
127	198	40	60	55.8	135031	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	242028	PASS
199	198	5	9	6.5	15790	PASS
275	198	10	30	18.8	45548	PASS
365	198	1	100	2.7	6494	PASS
441	443	0.01	100	80.6	18403	PASS
442	198	40	100	48.7	117901	PASS
443	442	17	23	19.4	22827	PASS