

Data File : H:\VOL1\GCMSDATA\J\121126\BJ001274.D
Acq On : 26 Nov 2012 13:33
Sample : P4-CCV
Misc : P4-CCV BNA_J HLM
MS Integration Params: RTEINT.P
Quant Time: Nov 26 16:48 2012

Vial: 2
Operator: HLM
Inst : BNA_J
Multiplr: 1.00

Instrument :
BNA_J
LabSampleId :
P4-CCV

Quant Results File: BJ111212.F

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)
Title : P4 by SOP M.5
Last Update : Mon Nov 26 16:48:06 2012
Response via : Initial Calibration
DataAcq Meth : P4

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.34	150	483327	2.50	ug/ml	0.00
System Monitoring Compounds						
2) Tripropylphosphate	6.44	99	409361	1.05	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	42.00%
Target Compounds						
3) White Phosphorus	4.71	124	388609	0.85	ug/ml	Ovalue 100

Quantitation Report


Data File : H:\VOL1\GCMSDATA\J\121126\BJ001274.D
 Acq On : 26 Nov 2012 13:33
 Sample : P4-CCV
 Misc : P4-CCV BNA_J HLM
 MS Integration Params: RTEINT.P
 Quant Time: Nov 26 16:48 2012




Vial: 2
 Operator: HLM
 Inst : BNA_J
 Multiplr: 1.00

Instrument :
 BNA_J
 LabSampleId :
 P4-CCV

Quant Results File: BJ111212.FILES

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M (RTE Integrator)
 Title : P4 by SOP M.5
 Last Update : Mon Nov 26 16:48:06 2012
 Response via : Initial Calibration

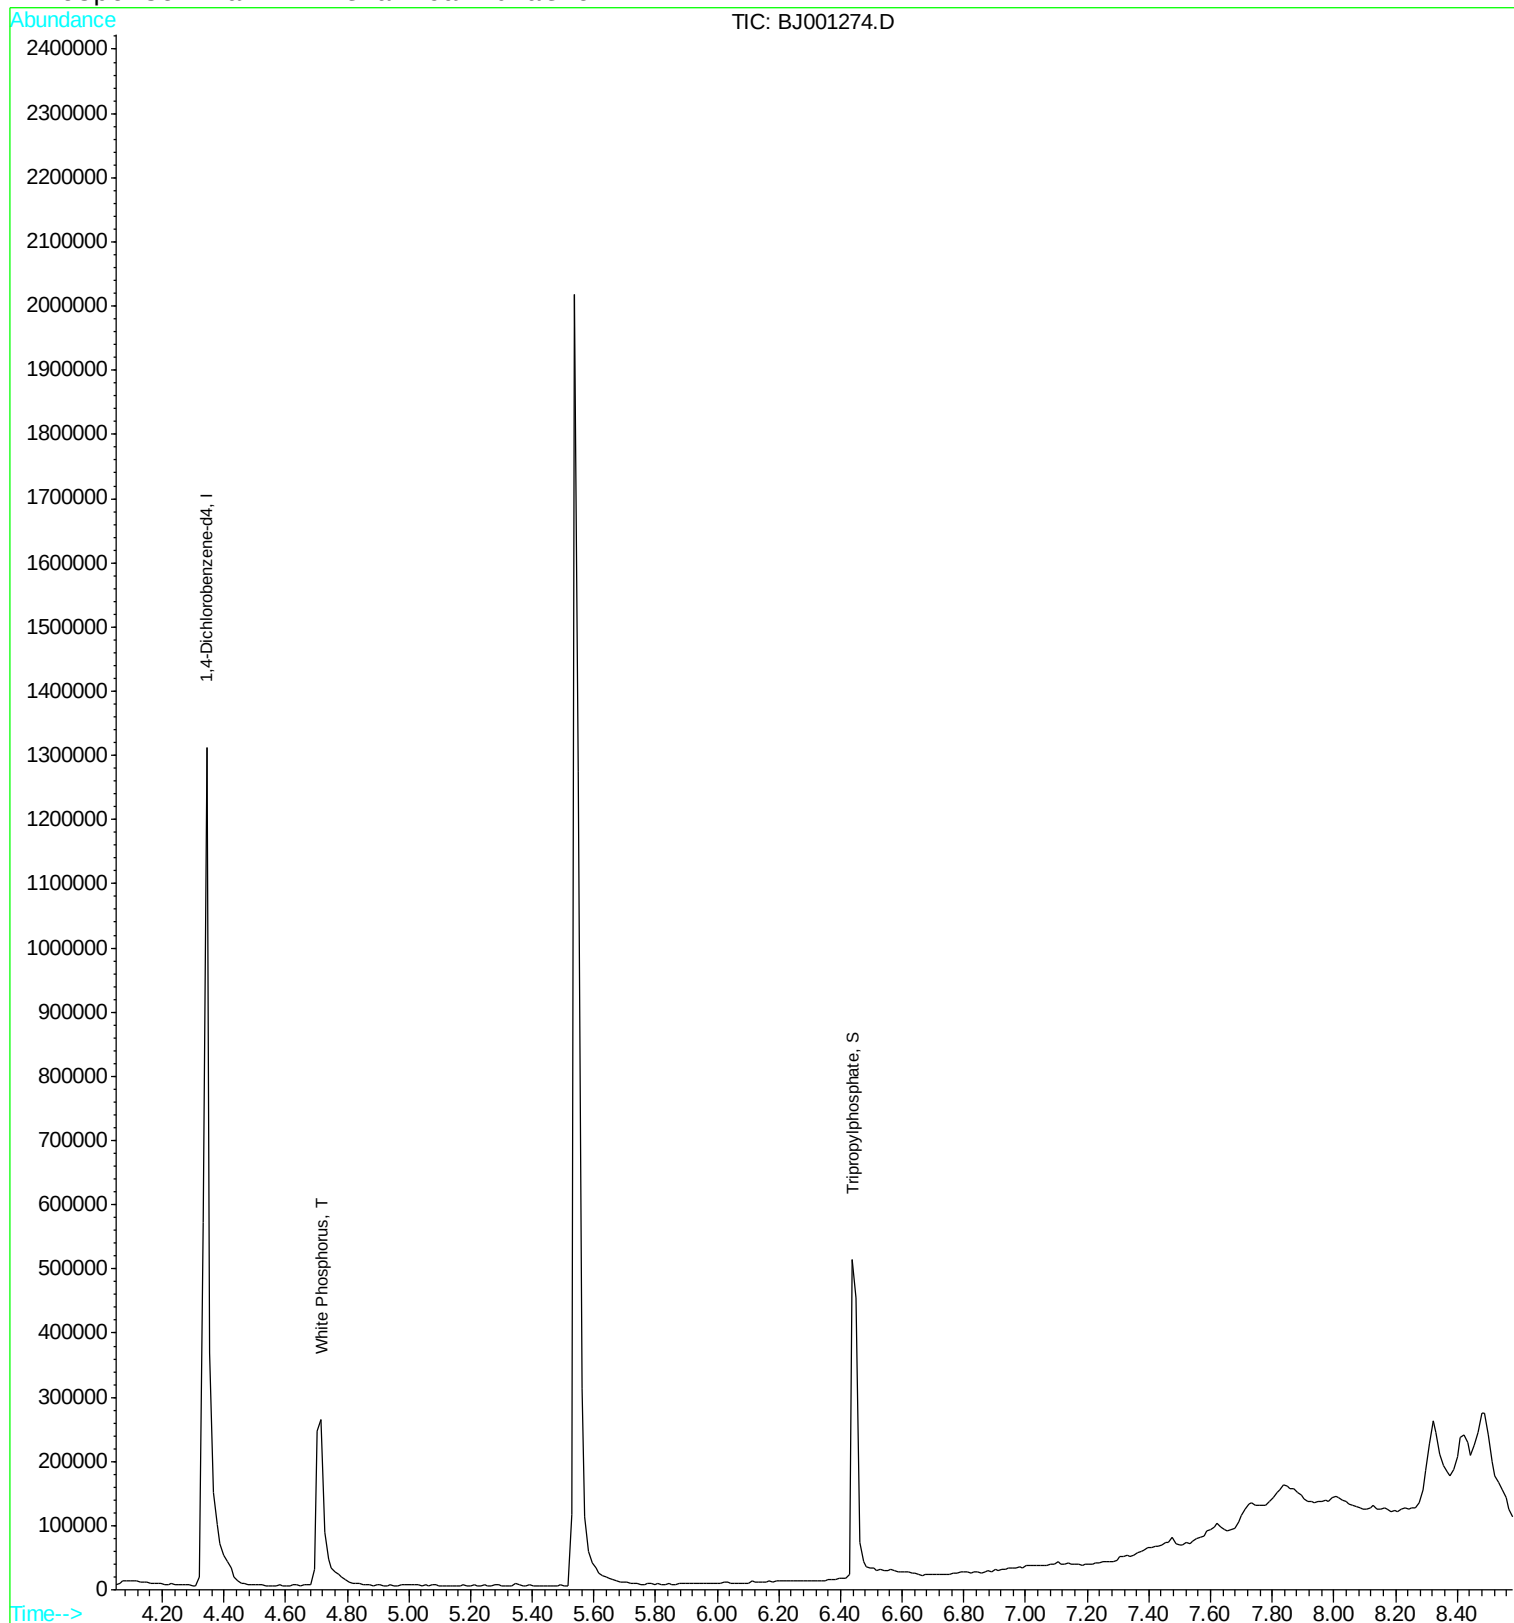

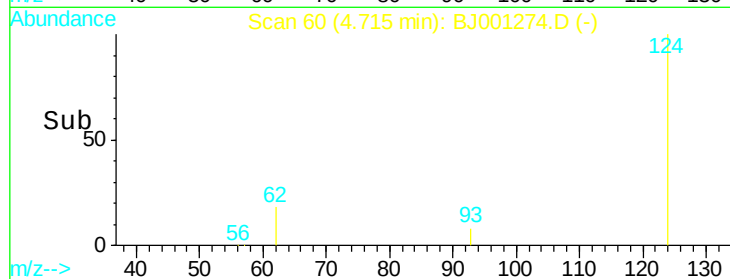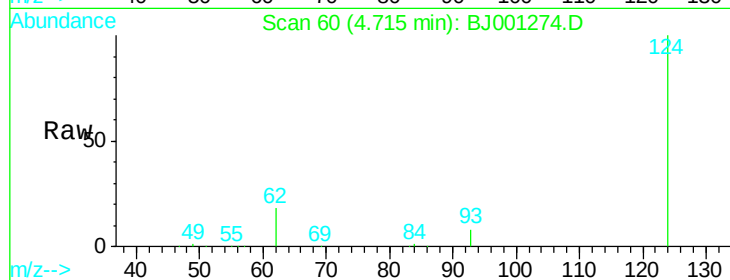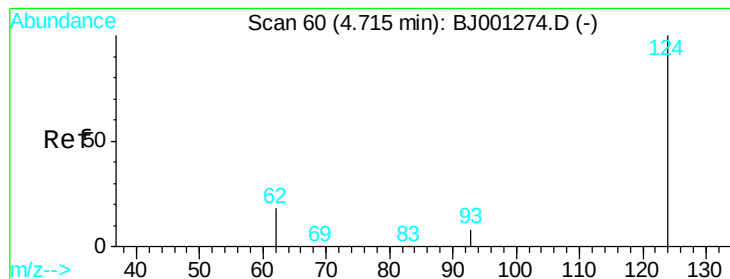

#3

White Phosphorus

Concen: 0.85 ug/ml

RT: 4.71 min Scan# 60

Delta R.T. 0.00 min

Lab File: BJ001274.D

Acq: 26 Nov 2012 13:33

Instrument :

BNA_J

LabSampleId :

P4-CCV

Tgt Ion:124 Resp: 388609

Ion Ratio Lower Upper

124 100

93 9.4 0.0 29.4

62 21.1 1.1 41.1

Abundance

Ion 124.00 (123.70 to 124.70): E

Ion 93.00 (92.70 to 93.70): BJ0

Ion 62.00 (61.70 to 62.70): BJ0

