

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
Data File : BJ001267.D
Acq On : 26 Nov 2012 11:32
Operator : HLM
Sample : P4-CCV
Misc : P4-CCV BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :

Quant Time: Nov 27 02:38:32 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Nov 21 16:04:24 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.33	150	869778	2.50	ug/ml	-0.03

System Monitoring Compounds

2) Tripropylphosphate	6.43	99	833462	1.19	ug/ml	-0.05
Spiked Amount	2.500	Range	20 - 150	Recovery	=	47.60%


Target Compounds					Qvalue
3) White Phosphorus	4.71	124	903340	1.09	ug/ml 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
Data File : BJ001267.D
Acq On : 26 Nov 2012 11:32
Operator : HLM
Sample : P4-CCV
Misc : P4-CCV BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :

Quant Time: Nov 27 02:38:32 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Wed Nov 21 16:04:24 2012
Response via : Initial Calibration

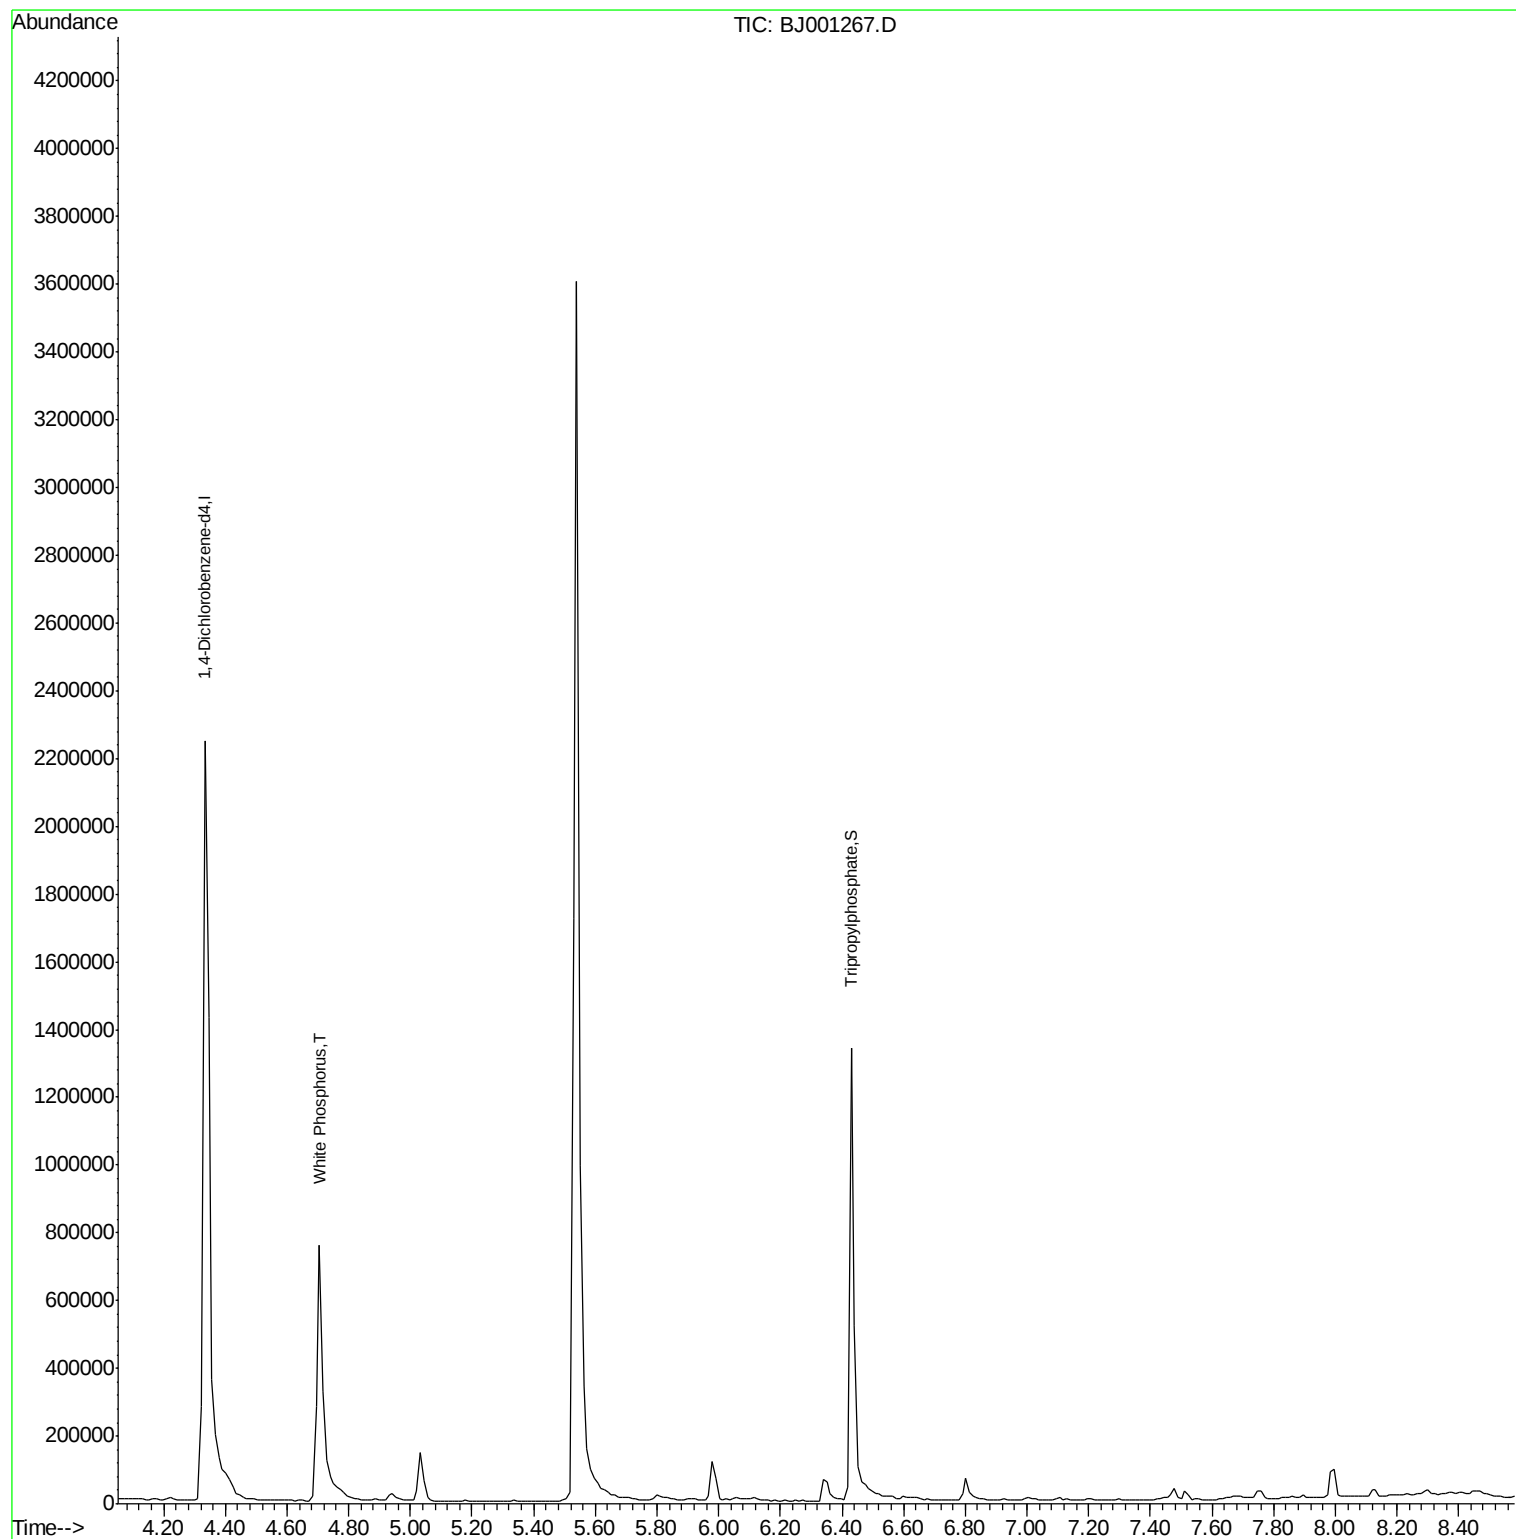




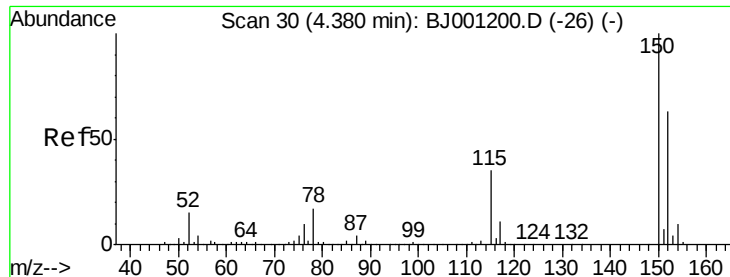


#1

1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.33 min Scan# 26
Delta R.T. -0.03 min
Lab File: BJ001267.D
Acq: 26 Nov 2012 11:32

Instrument :
BNA_J
ClientSampleId :




Tgt Ion:150 Resp: 869778
Ion Ratio Lower Upper
150 100
152 63.2 43.2 83.2

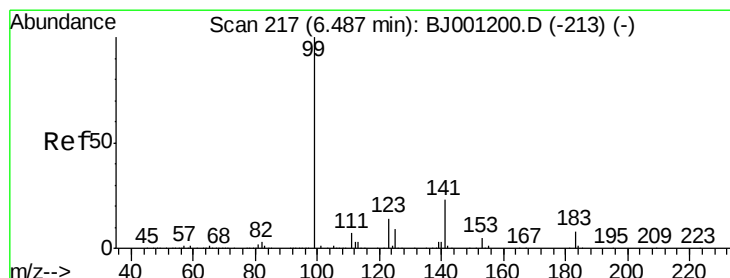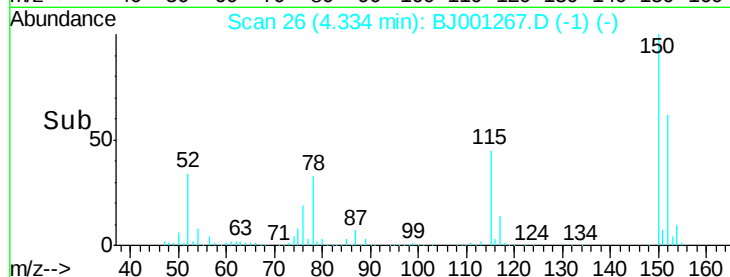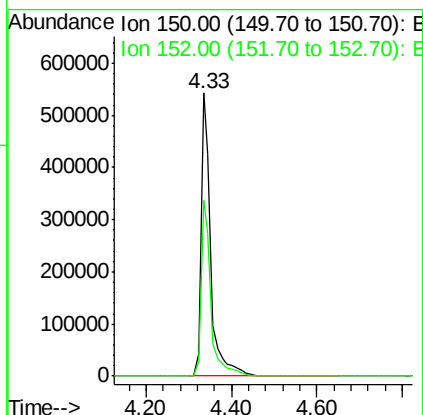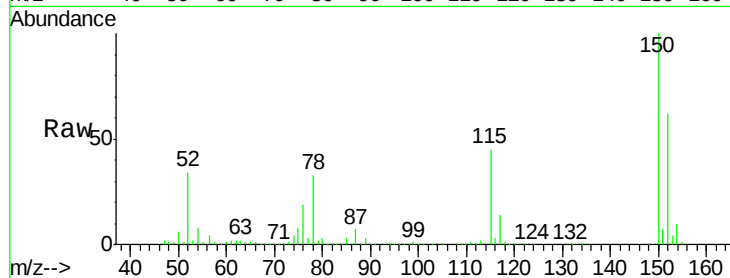


#2

Tripropylphosphate
Concen: 1.19 ug/ml
RT: 6.43 min Scan# 212
Delta R.T. -0.05 min
Lab File: BJ001267.D
Acq: 26 Nov 2012 11:32

Tgt Ion: 99 Resp: 833462
Ion Ratio Lower Upper
99 100
141 16.7 0.8 40.8

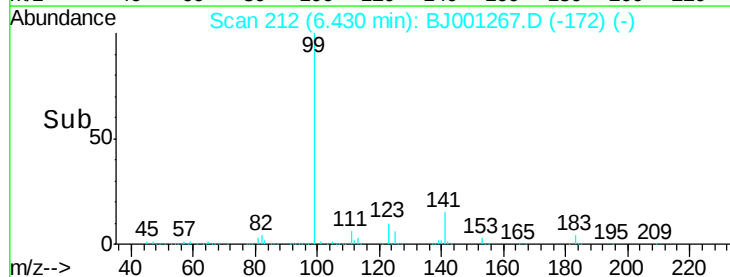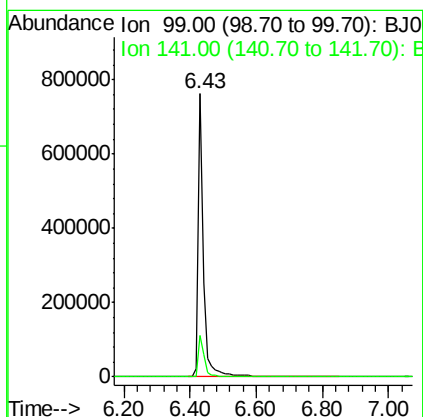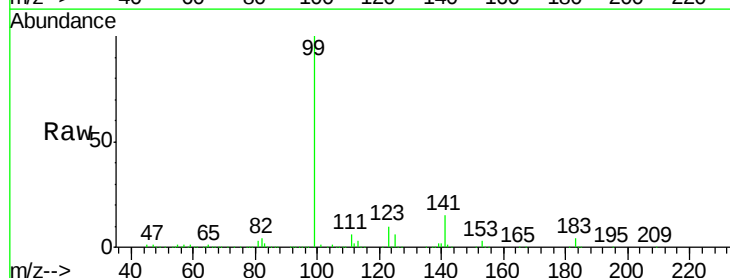

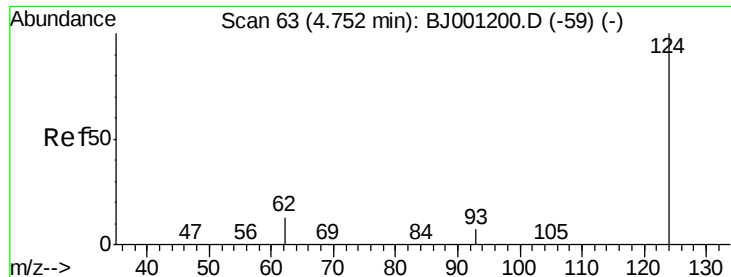

#3
 White Phosphorus
 Concen: 1.09 ug/ml
 RT: 4.71 min Scan# 59
 Delta R.T. -0.03 min
 Lab File: BJ001267.D
 Acq: 26 Nov 2012 11:32

Instrument :
 BNA_J
 ClientSampleId :

Tgt Ion:	124	Resp:	903340
Ion	Ratio	Lower	Upper
124	100		
93	9.7	0.0	28.6
62	22.3	0.0	38.9

