

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
Data File : BJ001274.D
Acq On : 26 Nov 2012 13:33
Operator : HLM
Sample : P4-CCV
Misc : P4-CCV BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-CCV

Quant Time: Nov 28 23:46:19 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ11212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 26 16:48:06 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.34	150	483327	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	6.44	99	409361	1.05	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	42.00%


Target Compounds					Qvalue
3) White Phosphorus	4.71	124	388609	0.85	ug/ml 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
Data File : BJ001274.D
Acq On : 26 Nov 2012 13:33
Operator : HLM
Sample : P4-CCV
Misc : P4-CCV BNA_J HLM
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_J
LabSampleId :
P4-CCV

Quant Time: Nov 28 23:46:19 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 26 16:48:06 2012
Response via : Initial Calibration

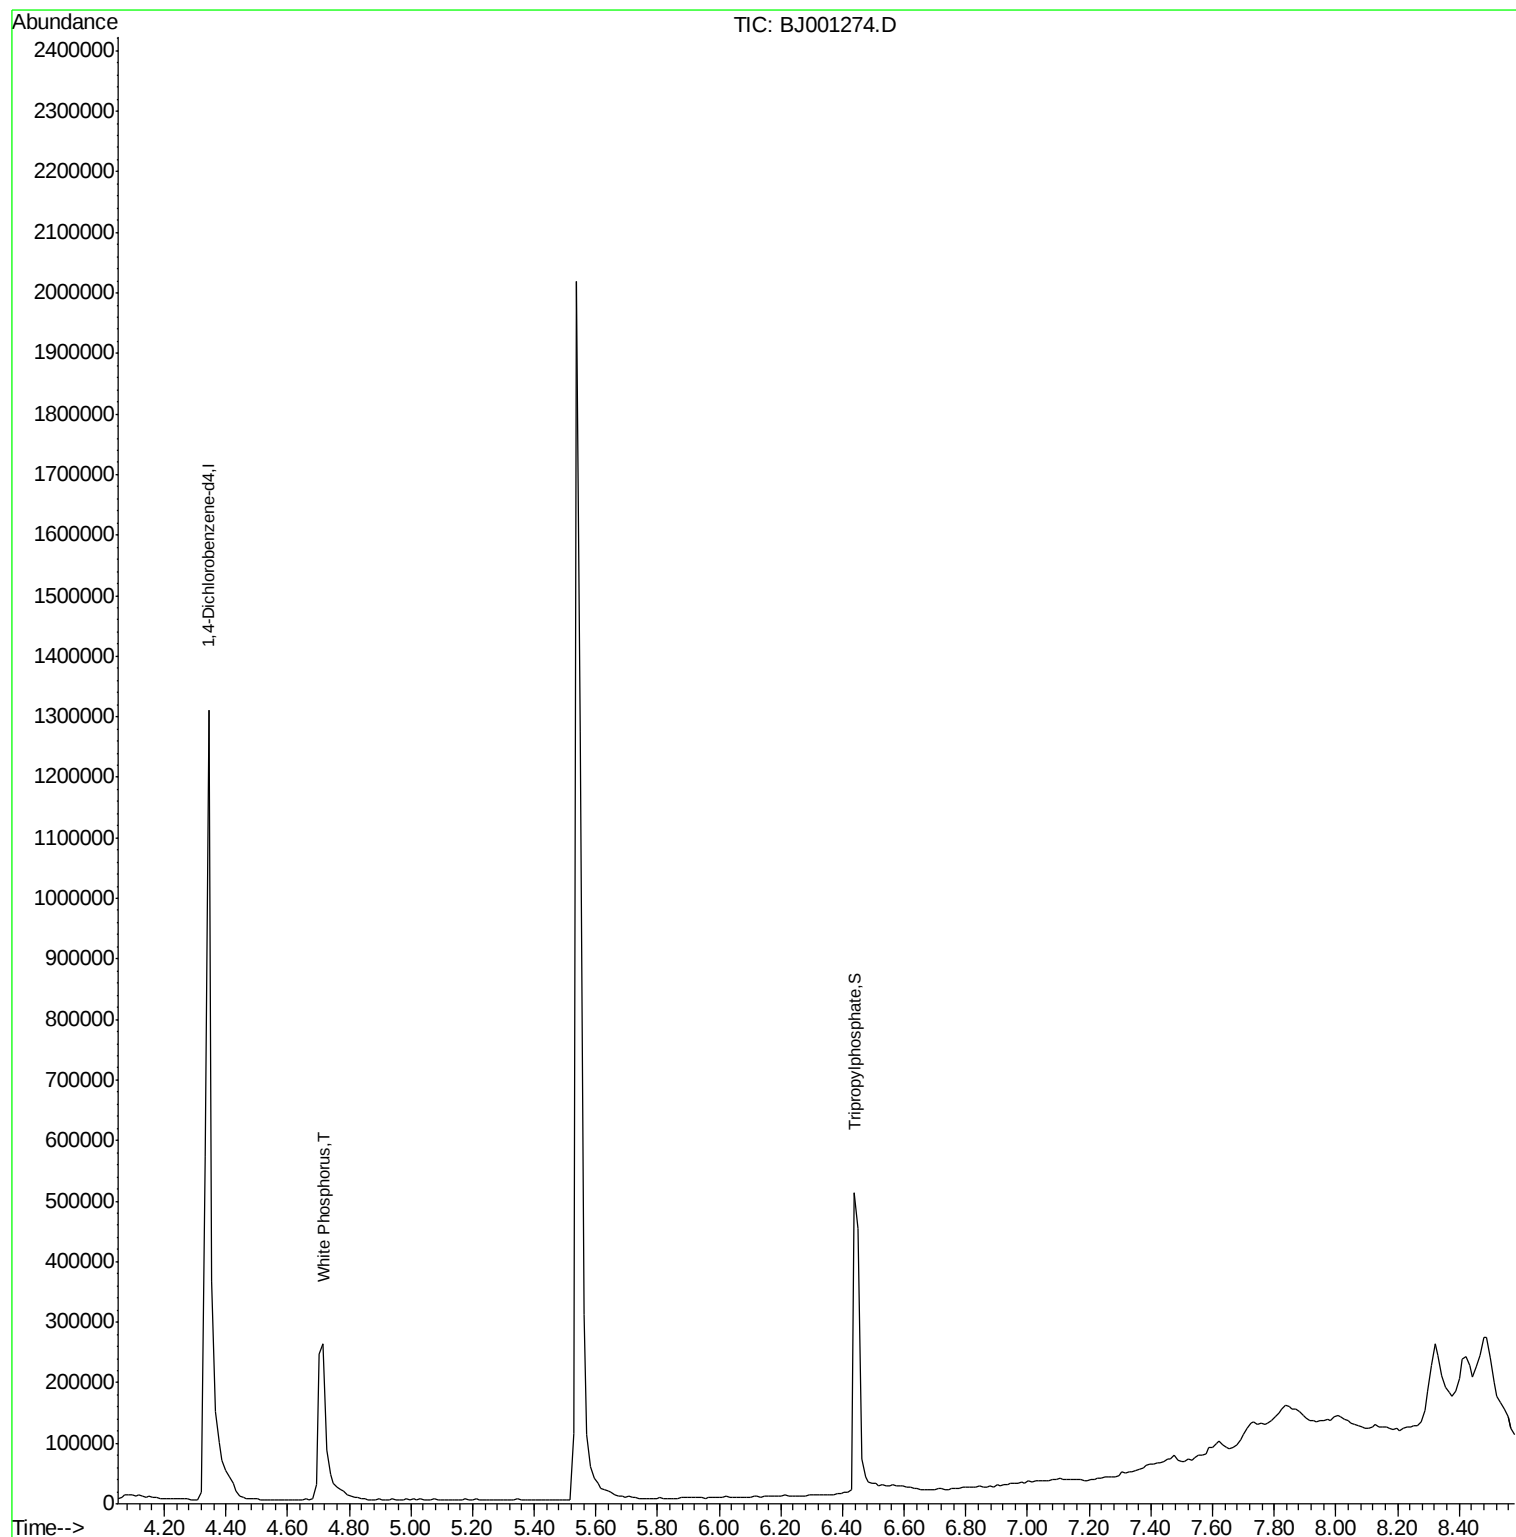

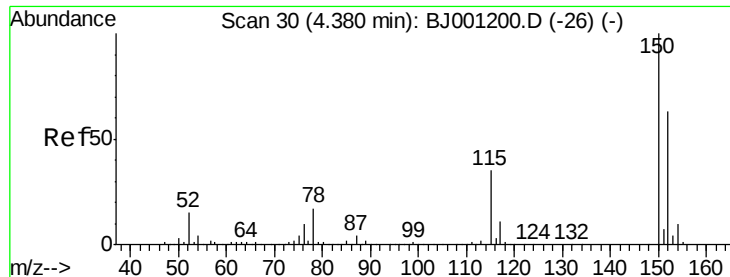


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.34 min Scan# 27
Delta R.T. 0.00 min
Lab File: BJ001274.D
Acq: 26 Nov 2012 13:33

Instrument :
BNA_J
LabSampleId :
P4-CCV

Tgt Ion:150 Resp: 483327
Ion Ratio Lower Upper
150 100
152 63.3 43.3 83.3

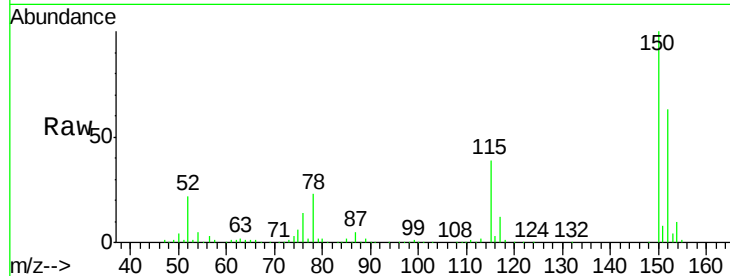


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

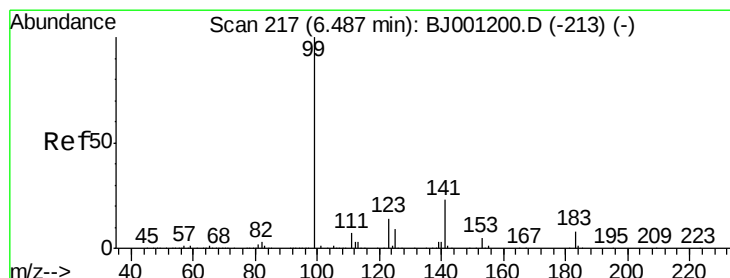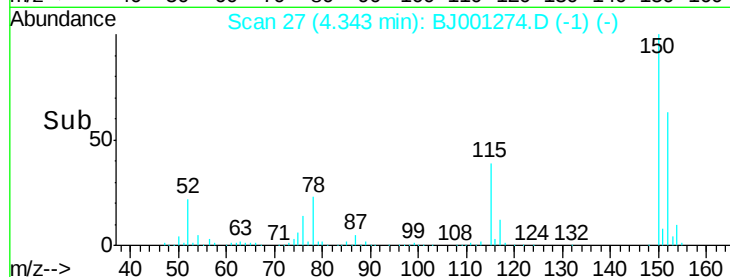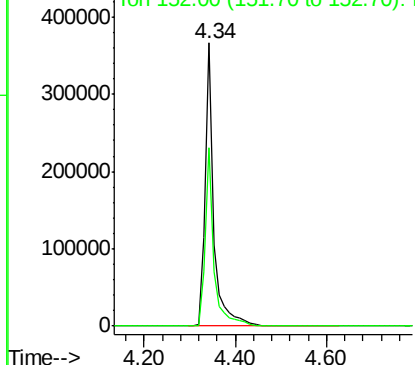



#2


Tripropylphosphate
Concen: 1.05 ug/ml
RT: 6.44 min Scan# 213
Delta R.T. 0.00 min
Lab File: BJ001274.D
Acq: 26 Nov 2012 13:33

Tgt Ion: 99 Resp: 409361
Ion Ratio Lower Upper
99 100
141 16.8 0.0 36.8

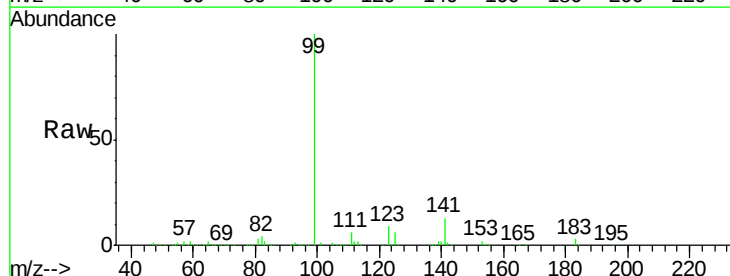

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

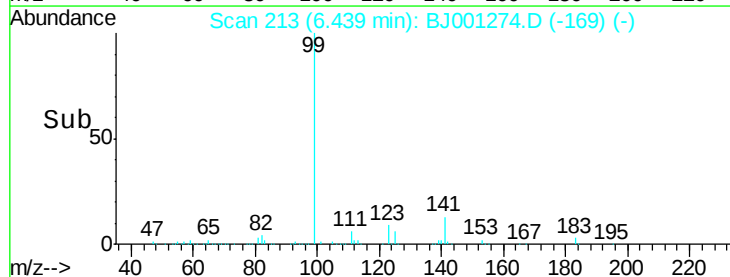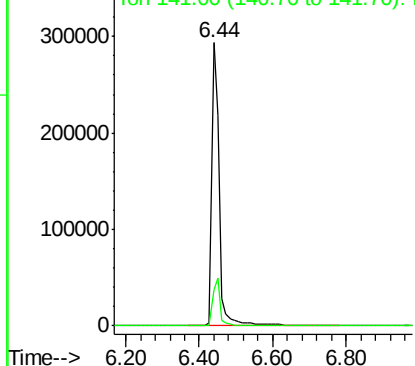

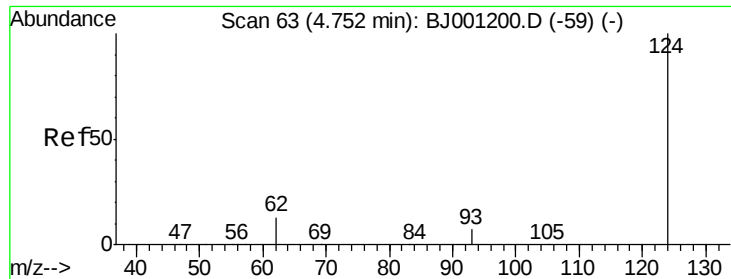

#3
 White Phosphorus
 Concen: 0.85 ug/ml
 RT: 4.71 min Scan# 60
 Delta R.T. 0.00 min
 Lab File: BJ001274.D
 Acq: 26 Nov 2012 13:33

Instrument :
 BNA_J
 LabSampleId :
 P4-CCV

Tgt Ion:	124	Resp:	388609
Ion	Ratio	Lower	Upper
124	100		
93	9.4	0.0	29.4
62	21.1	1.1	41.1

