

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
Data File : BJ001275.D
Acq On : 26 Nov 2012 13:57
Operator : HLM
Sample : PB66943BL
Misc : SOIL BNA_J HLM
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB66943BL

Quant Time: Nov 28 23:44:35 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 26 16:48:06 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.35	150	429793	2.50	ug/ml	0.00

System Monitoring Compounds

2) Tripropylphosphate	6.44	99	1065096	3.07	ug/ml	0.00
Spiked Amount	2.500	Range	20 - 150	Recovery	=	122.80%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
Data File : BJ001275.D
Acq On : 26 Nov 2012 13:57
Operator : HLM
Sample : PB66943BL
Misc : SOIL BNA_J HLM
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB66943BL

Quant Time: Nov 28 23:44:35 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 26 16:48:06 2012
Response via : Initial Calibration

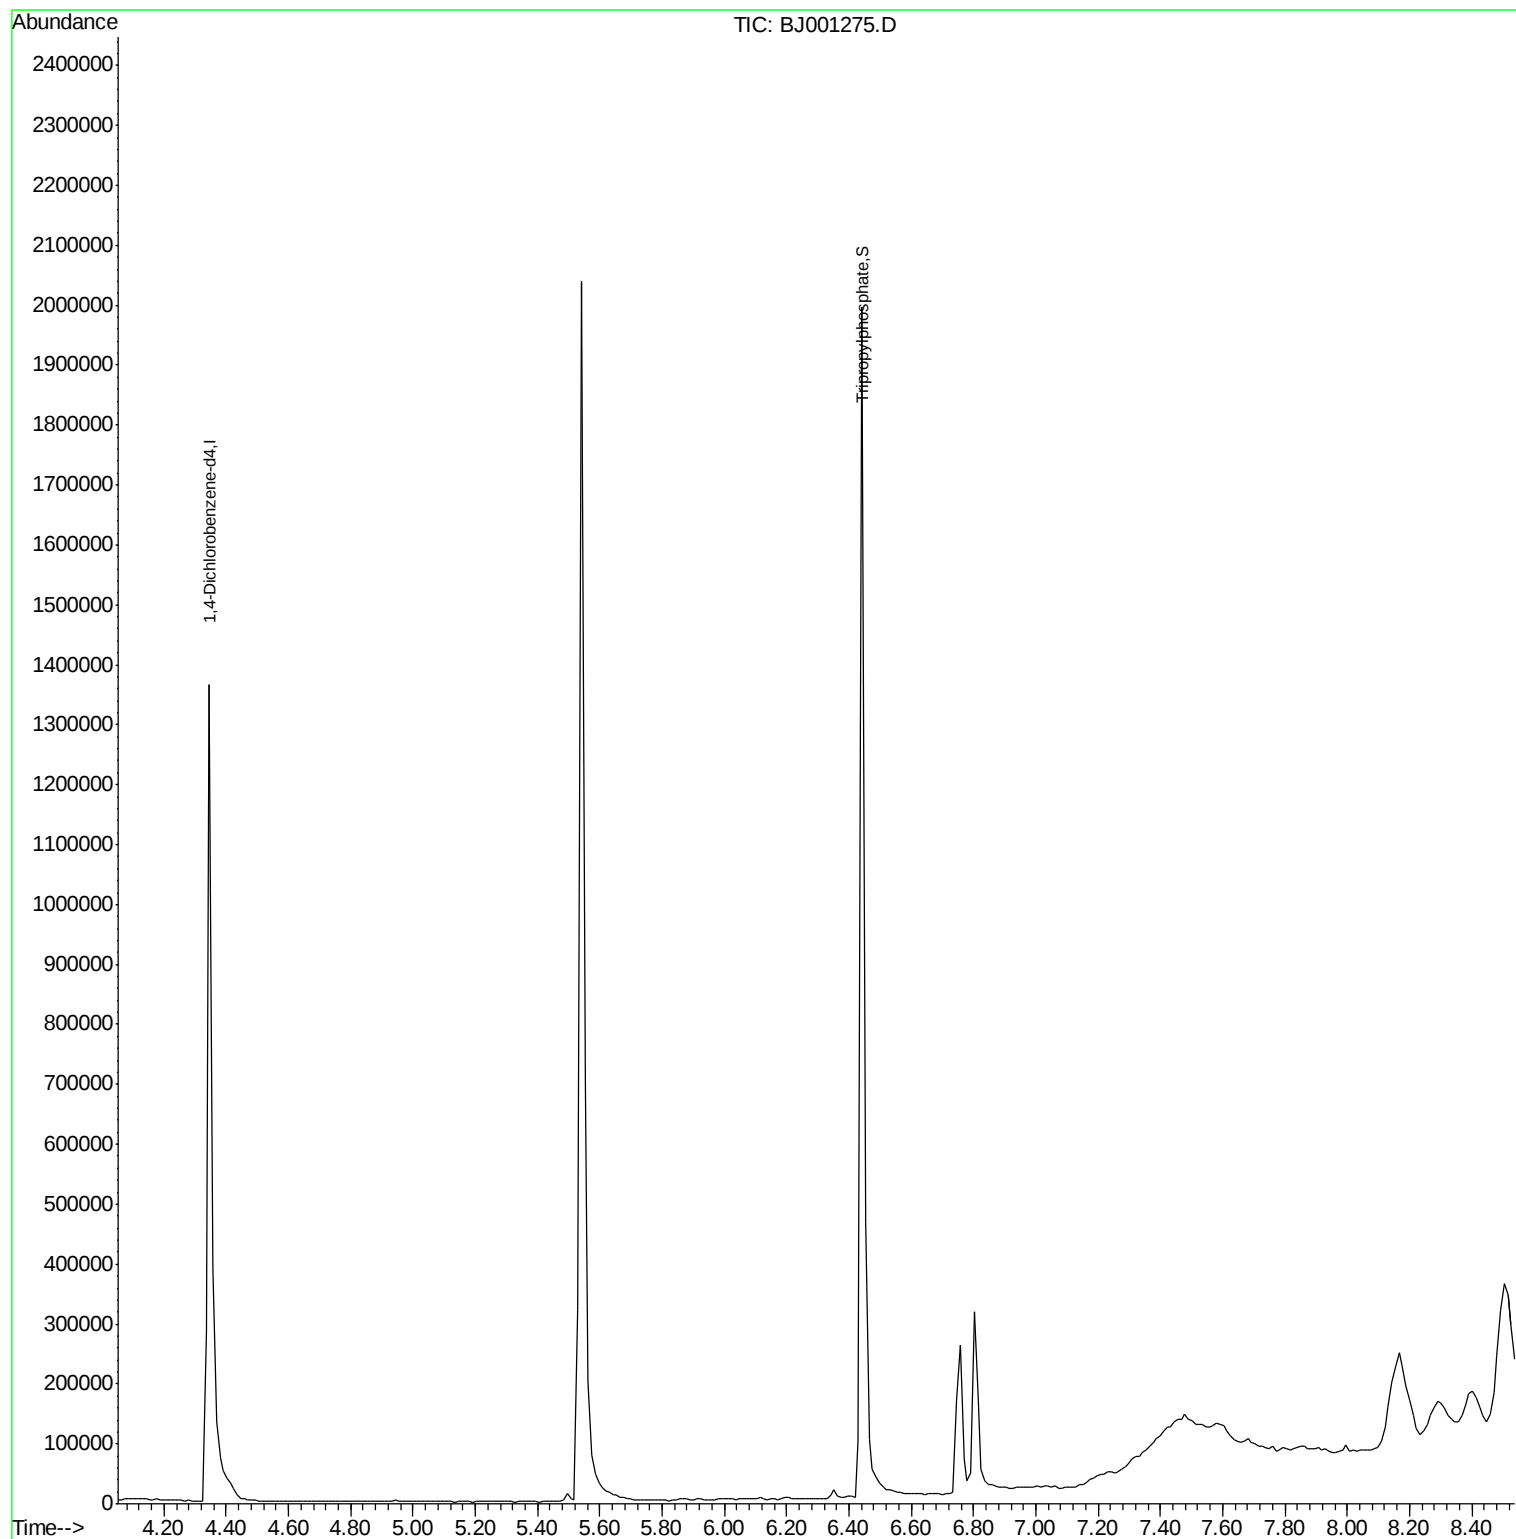

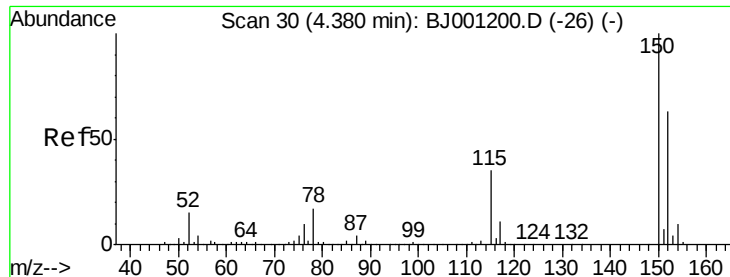

#1

1,4-Dichlorobenzene-d4

Concen: 2.50 ug/ml

RT: 4.35 min Scan# 27

Delta R.T. 0.00 min

Lab File: BJ001275.D

Acq: 26 Nov 2012 13:57

Instrument :

BNA_J

ClientSampleId :


PB66943BL

Tgt Ion:150 Resp: 429793

Ion Ratio Lower Upper

150 100

152 64.2 43.3 83.3

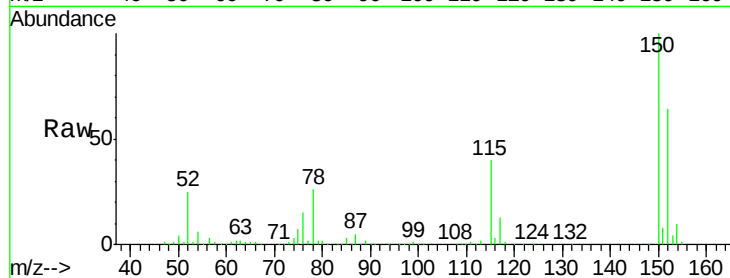

Abundance Ion 150.00 (149.70 to 150.70): E

Ion 152.00 (151.70 to 152.70): E

4.35

400000



300000

200000

100000

0

Time--> 4.20 4.40 4.60

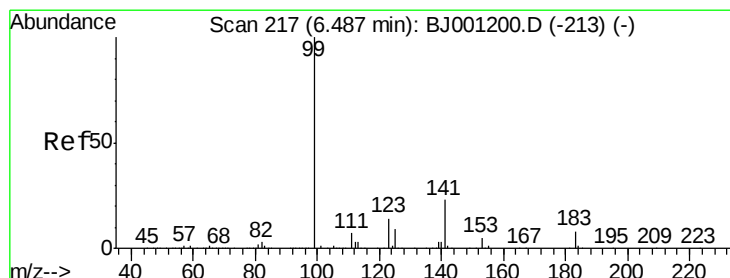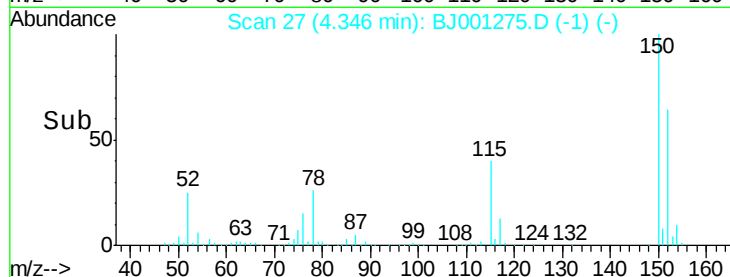

#2

Tripropylphosphate

Concen: 3.07 ug/ml

RT: 6.44 min Scan# 213

Delta R.T. 0.00 min

Lab File: BJ001275.D


Acq: 26 Nov 2012 13:57

Tgt Ion: 99 Resp: 1065096

Ion Ratio Lower Upper

99 100

141 16.8 0.0 36.8

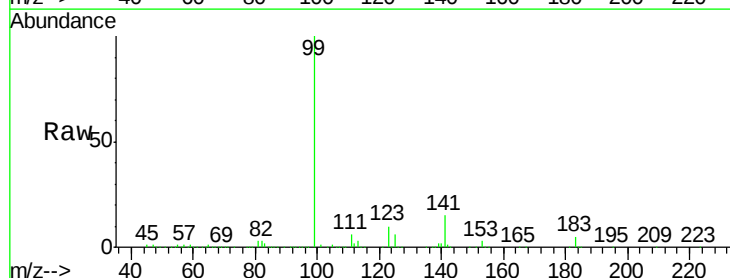

Abundance Ion 99.00 (98.70 to 99.70): BJ0

Ion 141.00 (140.70 to 141.70): E

6.44

1200000

1000000

800000

600000

400000

200000

0

Time--> 6.40 6.60 6.80

