

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
Data File : BJ001279.D
Acq On : 26 Nov 2012 14:50
Operator : HLM
Sample : D4844-01MSD
Misc : SOIL BNA_J HLM
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
LC522-01-SS01-AMSD

Quant Time: Nov 29 00:05:12 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 26 16:48:06 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.34	150	406092	2.50	ug/ml	0.00

System Monitoring Compounds
2) Tripropylphosphate 6.45 99 852608 2.60 ug/ml 0.00
Spiked Amount 2.500 Range 20 - 150 Recovery = 104.00%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) White Phosphorus	4.71	124	101001	0.26	ug/ml	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
Data File : BJ001279.D
Acq On : 26 Nov 2012 14:50
Operator : HLM
Sample : D4844-01MSD
Misc : SOIL BNA_J HLM
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
LC522-01-SS01-AMSD

Quant Time: Nov 29 00:05:12 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ11212.M
Quant Title : P4 by SOP M.5
QLast Update : Mon Nov 26 16:48:06 2012
Response via : Initial Calibration

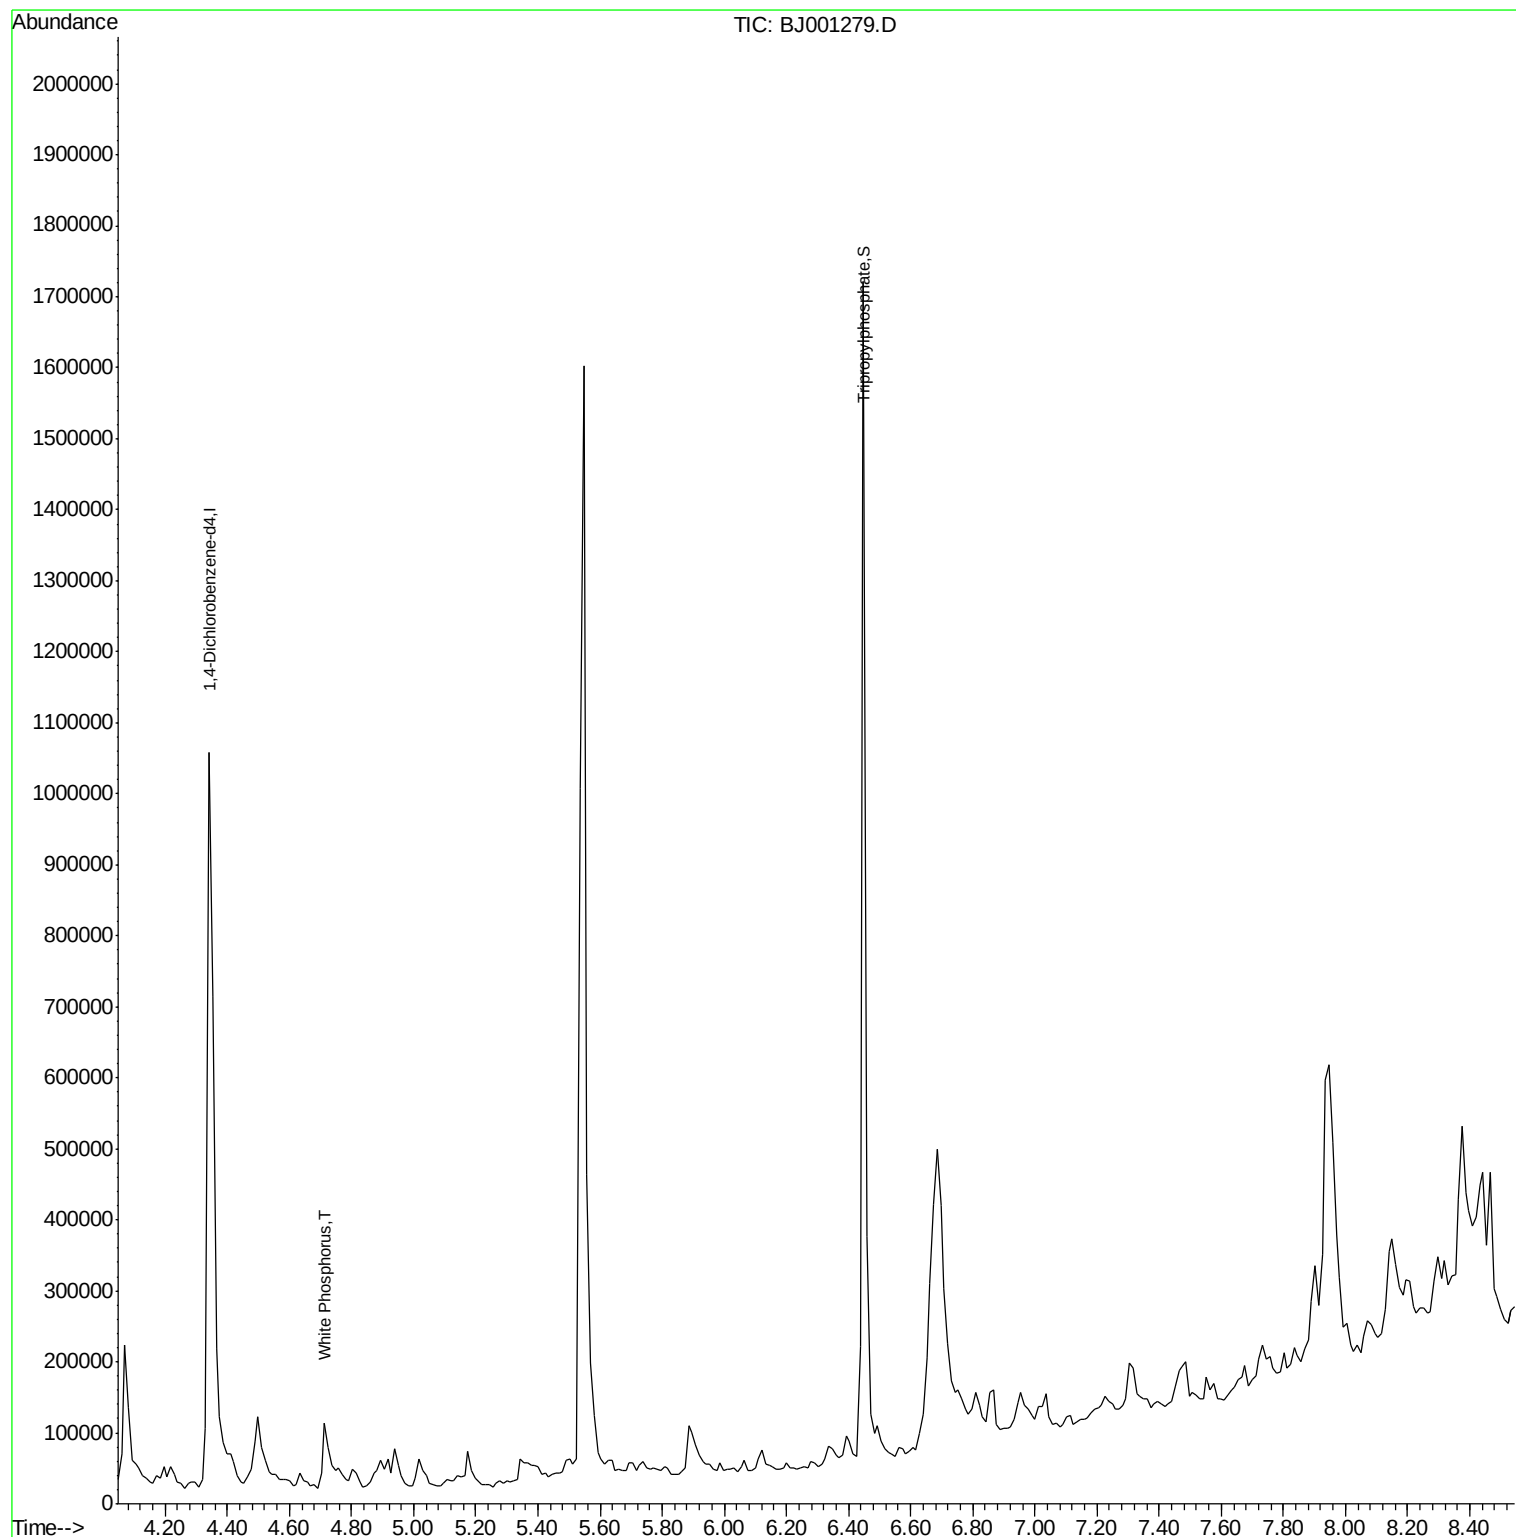

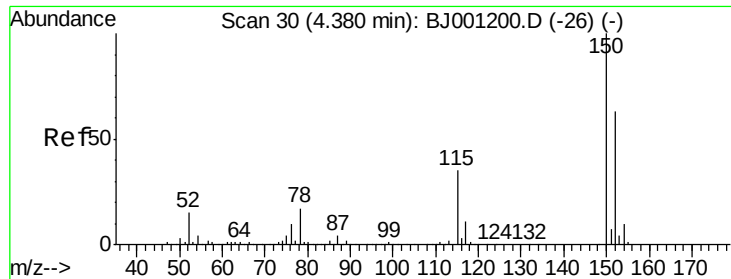


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/ml
RT: 4.34 min Scan# 27
Delta R.T. -0.00 min
Lab File: BJ001279.D
Acq: 26 Nov 2012 14:50

Instrument :
BNA_J
ClientSampleId :
LC522-01-SS01-AMSD

Tgt Ion:150 Resp: 406092
Ion Ratio Lower Upper
150 100
152 63.5 43.3 83.3

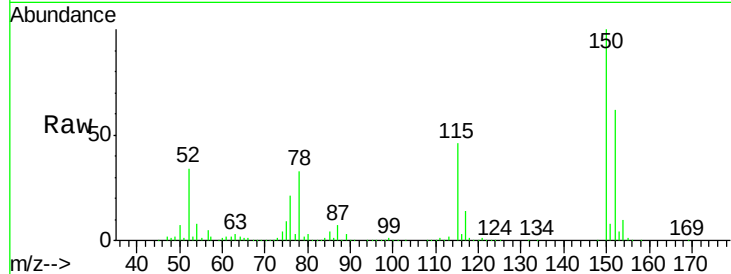


Abundance Ion 150.00 (149.70 to 150.70): E
Ion 152.00 (151.70 to 152.70): E

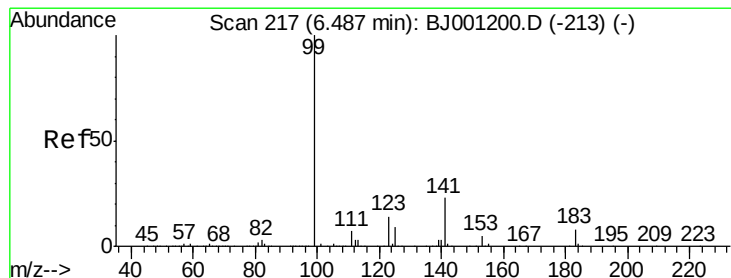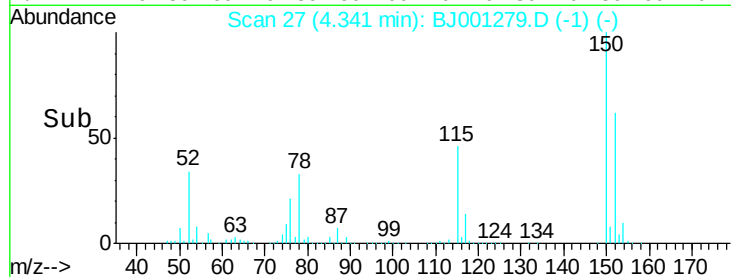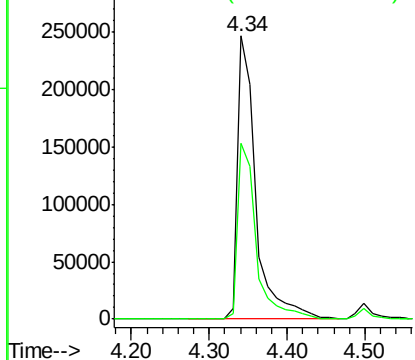



#2


Tripropylphosphate
Concen: 2.60 ug/ml
RT: 6.45 min Scan# 214
Delta R.T. 0.01 min
Lab File: BJ001279.D
Acq: 26 Nov 2012 14:50

Tgt Ion: 99 Resp: 852608
Ion Ratio Lower Upper
99 100
141 17.6 0.0 36.8

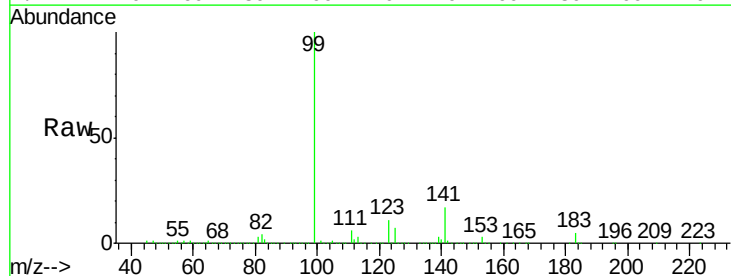

Abundance Ion 99.00 (98.70 to 99.70): BJ0
Ion 141.00 (140.70 to 141.70): E

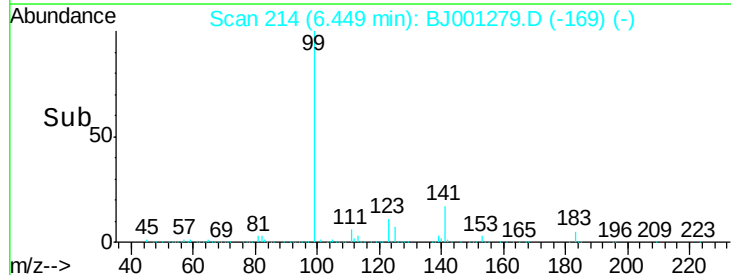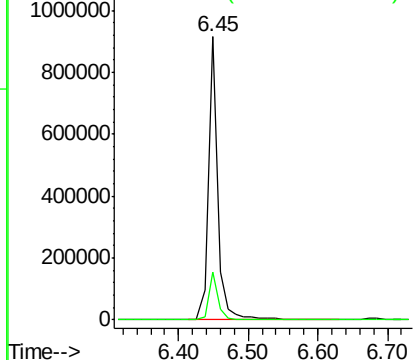

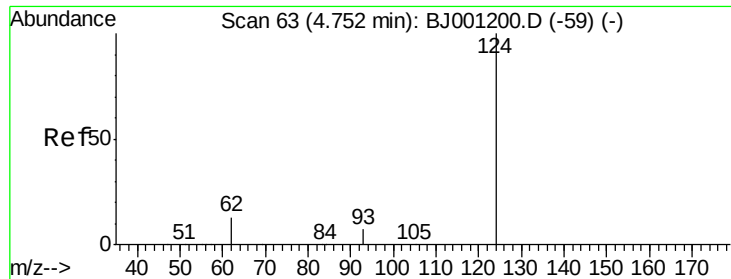

#3
 White Phosphorus
 Concen: 0.26 ug/ml
 RT: 4.71 min Scan# 60
 Delta R.T. -0.00 min
 Lab File: BJ001279.D
 Acq: 26 Nov 2012 14:50

Instrument :
 BNA_J
 ClientSampleId :
 LC522-01-SS01-AMSD

Tgt Ion	Ratio	Lower	Upper
124	100		
93	9.6	0.0	29.4
62	22.7	1.1	41.1

