

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
 Data File : BJ001282.D
 Acq On : 26 Nov 2012 15:29
 Operator : HLM
 Sample : D4844-04
 Misc : SOIL BNA_J HLM
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 LC521-01-SS02-A

Quant Time: Nov 29 00:05:22 2012
 Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ111212.M
 Quant Title : P4 by SOP M.5
 QLast Update : Mon Nov 26 16:48:06 2012
 Response via : Initial Calibration

| Internal Standards | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 4.34 | 150 | 369296 | 2.50 | ug/ml | 0.00 |

| | | | | | | |
|-----------------------------|-------|-------|----------|----------|-------|---------|
| System Monitoring Compounds | | | | | | |
| 2) Tripropylphosphate | 6.46 | 99 | 863111 | 2.90 | ug/ml | 0.02 |
| Spiked Amount | 2.500 | Range | 20 - 150 | Recovery | = | 116.00% |


| Target Compounds | Qvalue |
|------------------|--------|
| ----- | |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
 Data File : BJ001282.D
 Acq On : 26 Nov 2012 15:29
 Operator : HLM
 Sample : D4844-04
 Misc : SOIL BNA_J HLM
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_J
ClientSampled :
 LC521-01-SS02-A

Quant Time: Nov 29 00:05:22 2012
 Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ11212.M
 Quant Title : P4 by SOP M.5
 QLast Update : Mon Nov 26 16:48:06 2012
 Response via : Initial Calibration




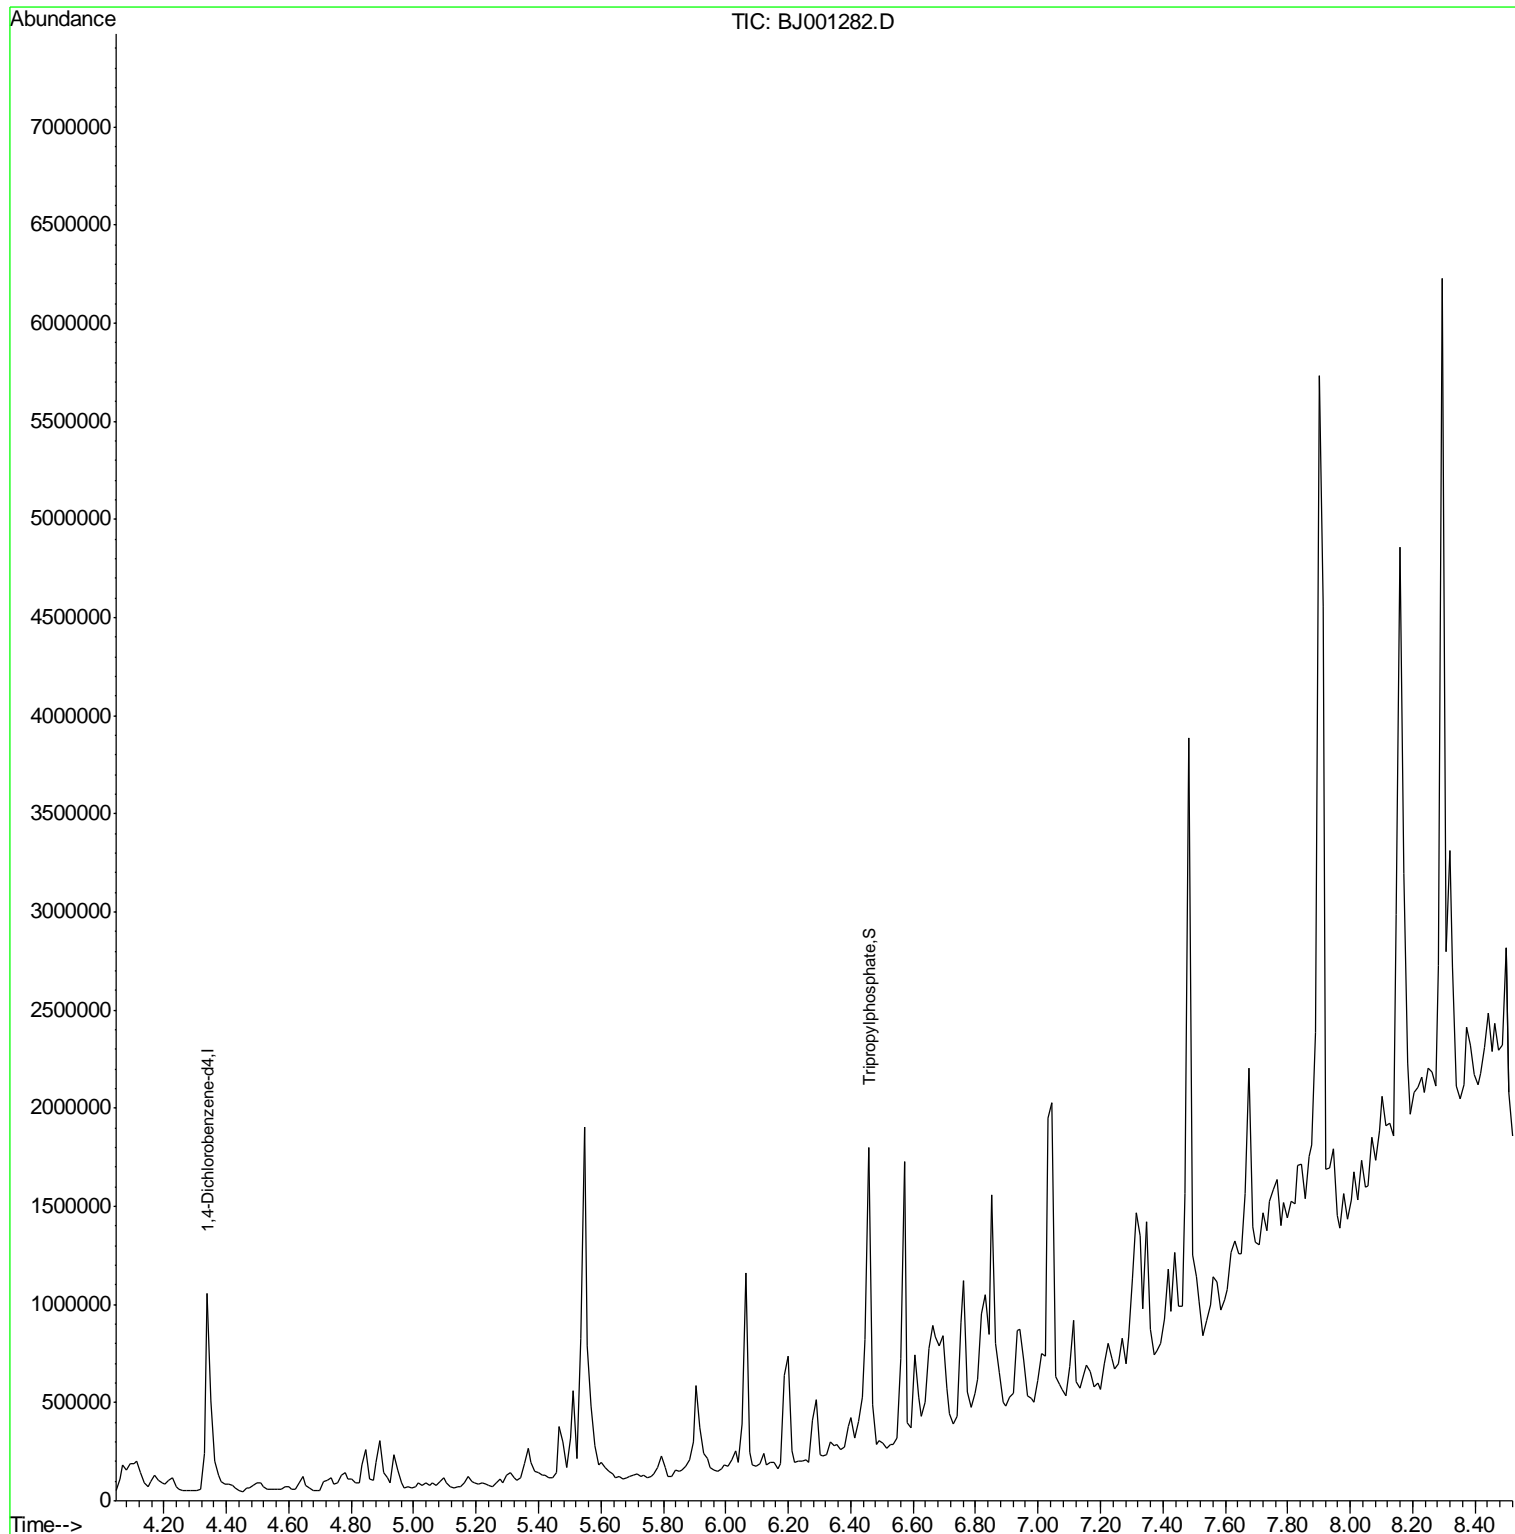


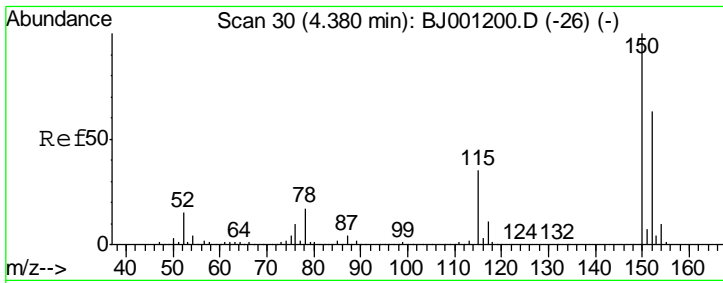

#1
 1,4-Dichlorobenzene-d4
 Concen: 2.50 ug/ml
 RT: 4.34 min Scan# 27
 Delta R.T. -0.00 min
 Lab File: BJ001282.D
 Acq: 26 Nov 2012 15:29

Instrument :
 BNA_J
 ClientSampleId :
 LC521-01-SS02-A

Tgt Ion: 150 Resp: 369296
 Ion Ratio Lower Upper
 150 100
 152 64.3 43.3 83.3

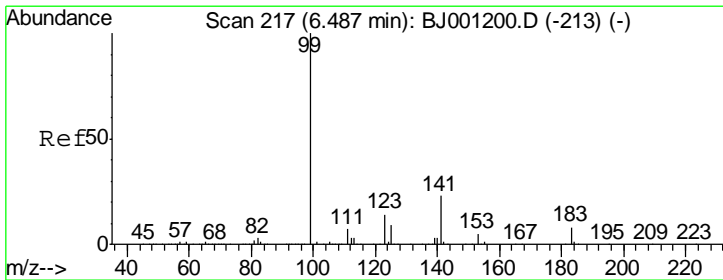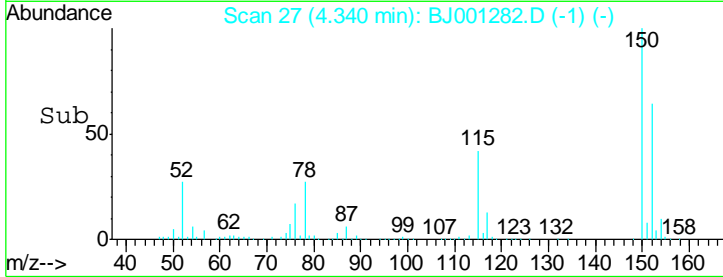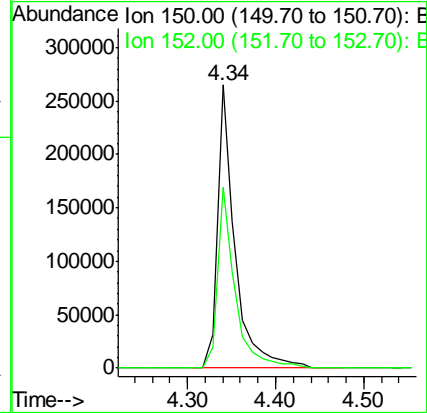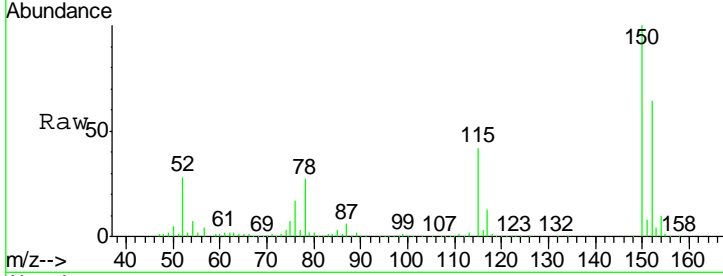

#2
 Tripropylphosphate
 Concen: 2.90 ug/ml
 RT: 6.46 min Scan# 215
 Delta R.T. 0.02 min
 Lab File: BJ001282.D
 Acq: 26 Nov 2012 15:29

Tgt Ion: 99 Resp: 863111
 Ion Ratio Lower Upper
 99 100
 141 16.7 0.0 36.8

