


Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112612\
 Data File : BJ001266.D
 Acq On : 26 Nov 2012 11:16
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_J\METHOD\BJ111212.M
 Title : P4 by SOP M.5
 Last Update : Mon Nov 12 15:57:06 2012

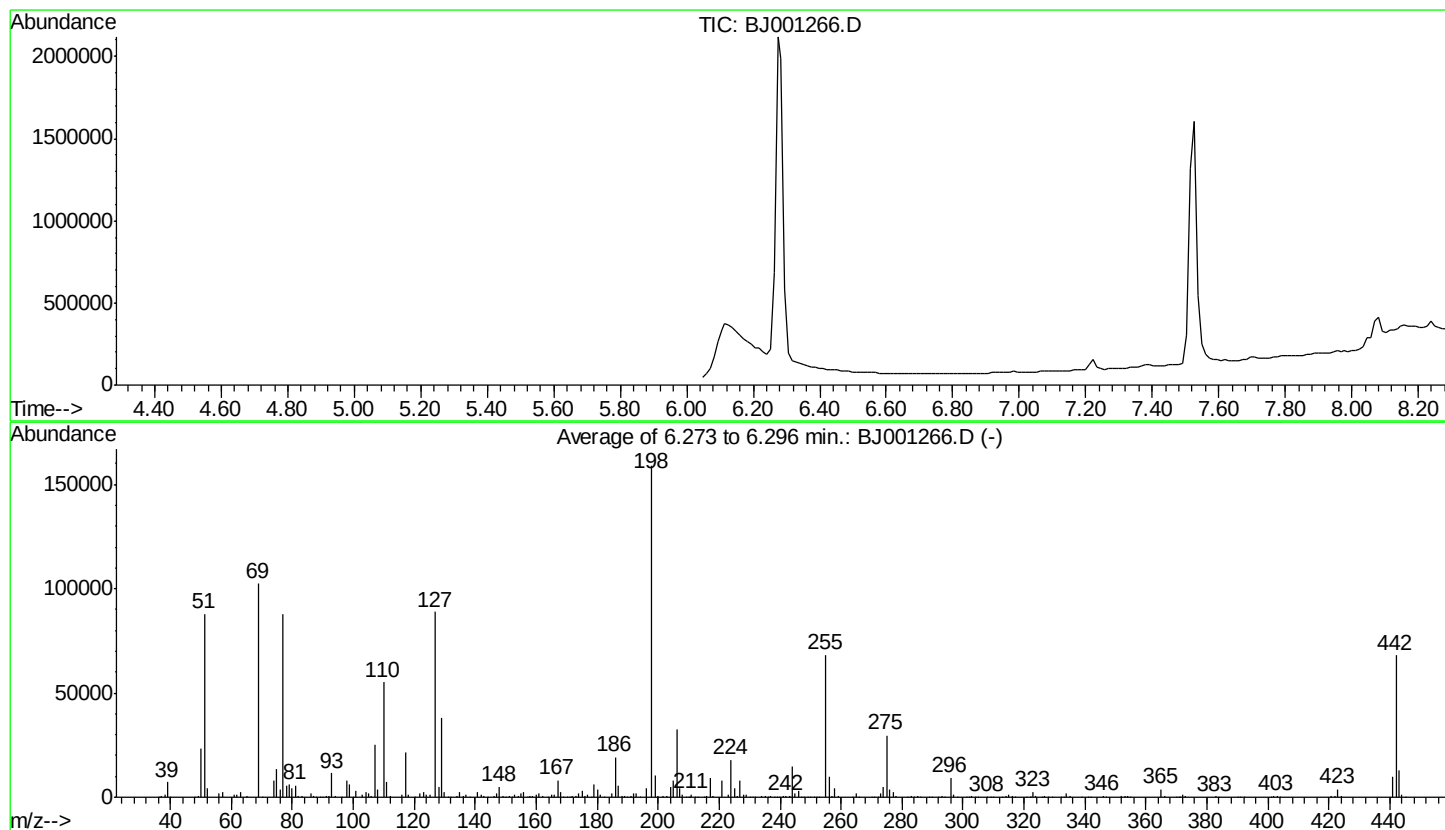

AutoFind: Scans 21, 22, 23; Background Corrected with Scan 13

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	55.4	88140	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	64.3	102312	PASS
70	69	0.00	2	0.0	35	PASS
127	198	40	60	55.9	88993	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	159091	PASS
199	198	5	9	6.5	10269	PASS
275	198	10	30	18.7	29705	PASS
365	198	1	100	2.5	3945	PASS
441	443	0.01	100	77.7	10147	PASS
442	198	40	100	42.7	67893	PASS
443	442	17	23	19.2	13065	PASS