

Data File : H:\VOL1\GCMSDATA\J\121127\BJ001302.D
 Acq On : 27 Nov 2012 16:48
 Sample : D4921-03
 Misc : WATER BNA J HLM
 MS Integration Params: rteint.p
 Quant Time: Nov 28 14:03 2012

Vial: 14
 Operator: HLM
 Inst : BNA J
 Multiplr: 1.00

Instrument :
 BNA_J
 ClientSampleId :
 CC23A-112012F

Quant Results File: BJ112712.F

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M (RTE Integrator)
 Title : CWA degradation products by GCMS
 Last Update : Tue Nov 27 14:50:43 2012
 Response via : Initial Calibration
 DataAcq Meth : CWAJ

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	152	324305	2.50	ug/mL	0.00
6) Naphthalene-d8	5.63	136	1335318	2.50	ug/mL	0.00
System Monitoring Compounds						
10) Tripropylphosphate	6.71	99	243596	0.46	ug/mL	0.00
Spiked Amount 0.500	Range	70 - 130	Recovery	=	92.00%	
12) 2-Bromothioanisole	6.92	204	347460	3.91	ug/mL	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	78.20%	
Target Compounds						
9) Benzothiazole	5.92	135	2999	0.01	ug/mL#	1
14) p-Chlorophenylmethanesulfon	7.74	111	4562	0.02	ug/mL#	38

Data File : H:\VOL1\GCMSDATA\J\121127\BJ001302.D

Vial: 14

Acq On : 27 Nov 2012 16:48

Operator: HLM

Sample : D4921-03

Inst : BNA J

Misc : WATER BNA J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Nov 28 14:03 2012

Quant Results File: BJ112712.RES

Instrument :

BNA_J

ClientSampleId :


CC23A-112012F


Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M (RTE Integrator)

Title : CWA degradation products by GCMS

Last Update : Tue Nov 27 14:50:43 2012

Response via : Initial Calibration

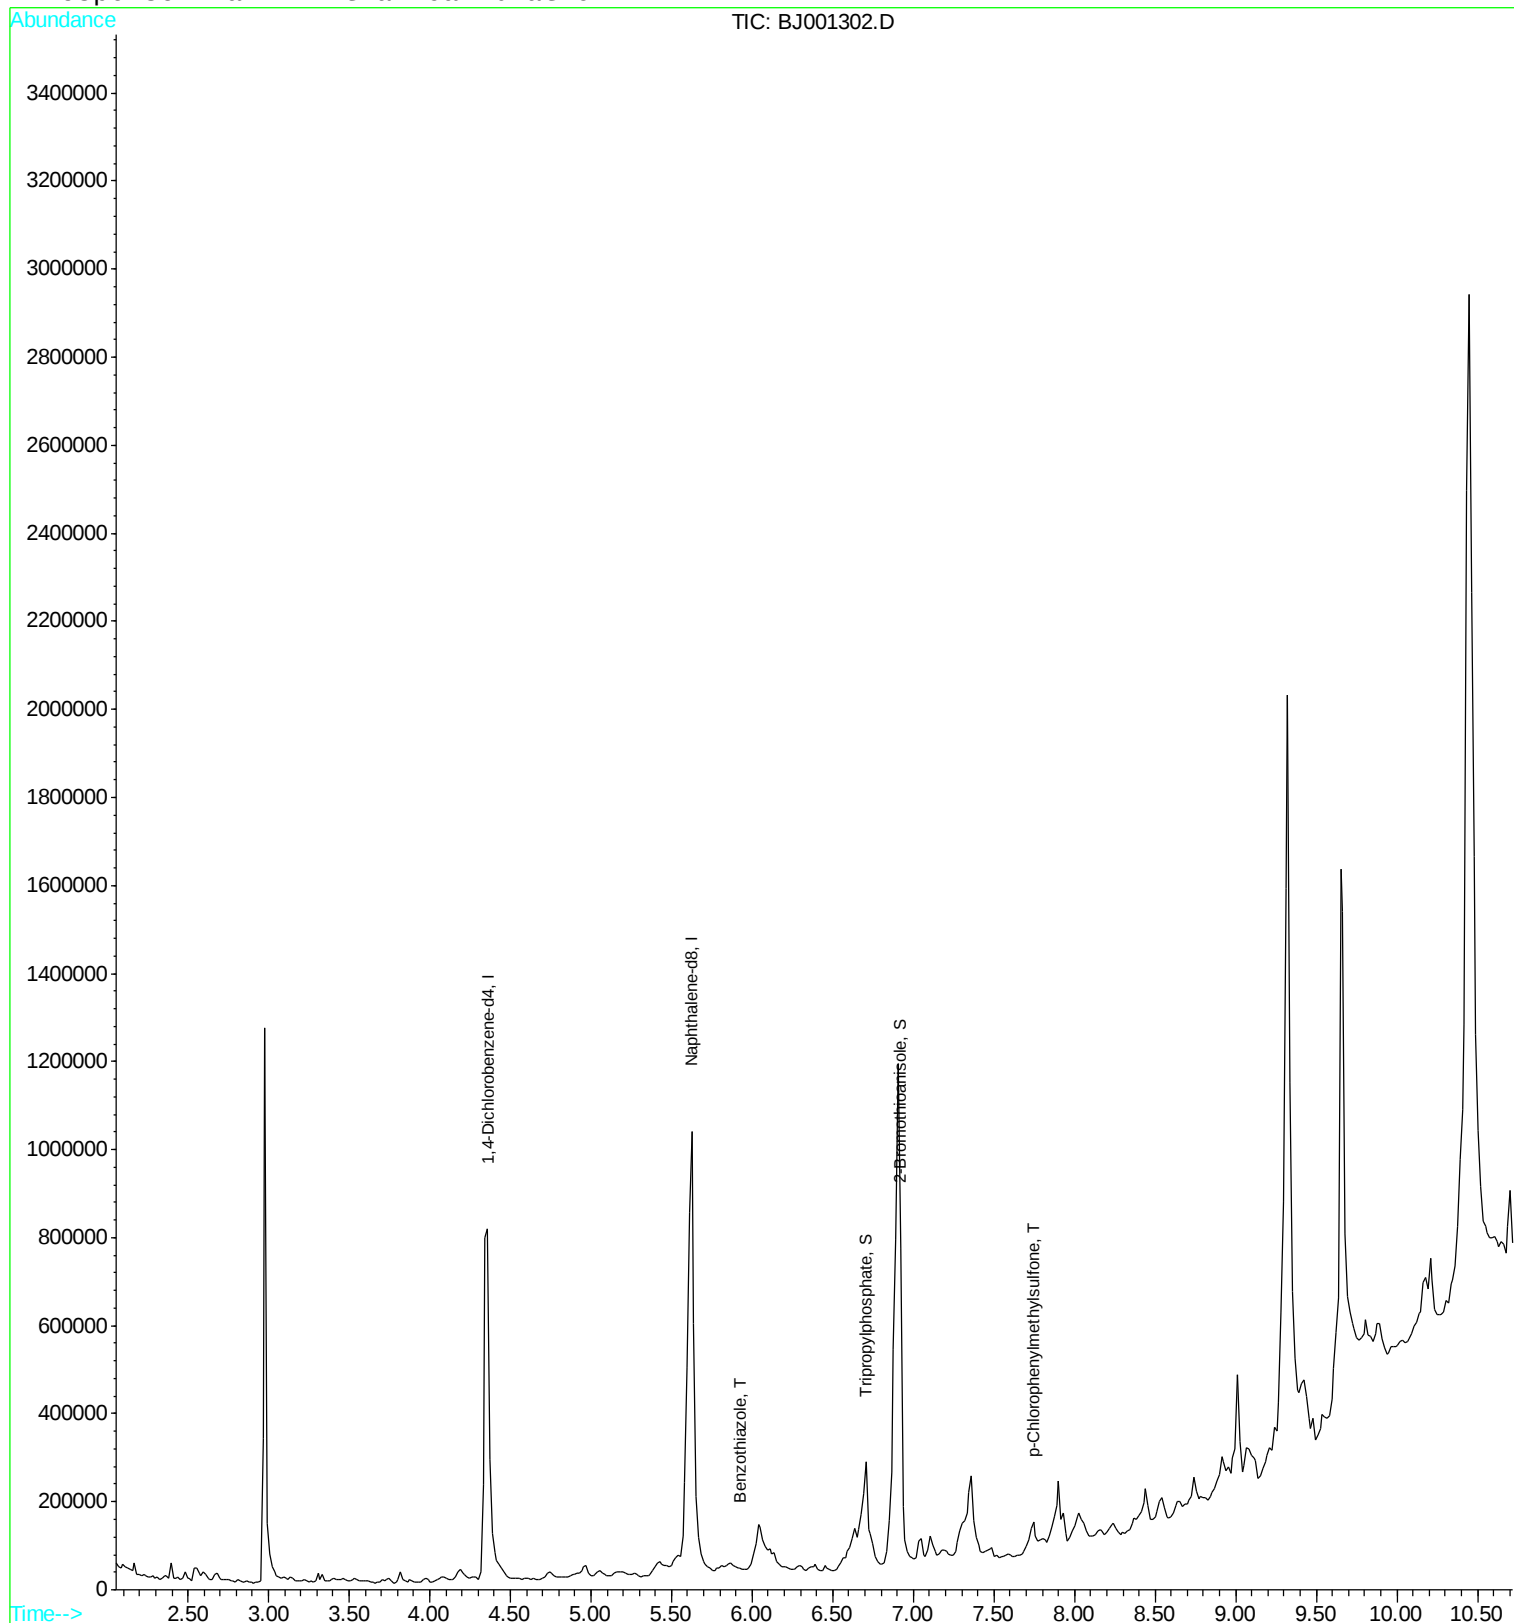

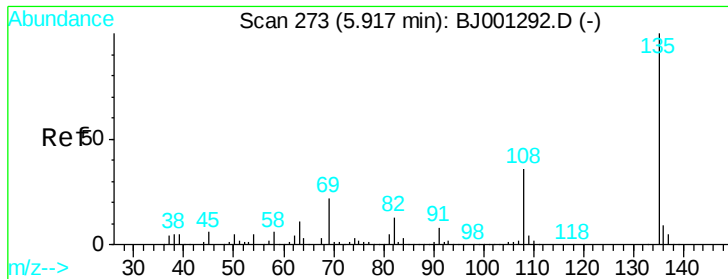

#9

Benzothiazole

Concen: 0.01 ug/mL

RT: 5.92 min Scan# 273

Delta R.T. 0.01 min

Lab File: BJ001302.D

Acq: 27 Nov 2012 16:48

Instrument :

BNA_J

ClientSampleId :

CC23A-112012F


Tgt Ion:135 Resp: 2999

Ion Ratio Lower Upper

135 100

108 51.8 15.7 55.7

69 145.5 2.2 42.2#



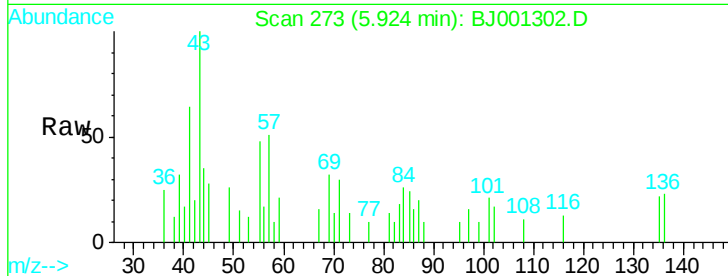


Abundance

Ion 135.00 (134.70 to 135.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 69.00 (68.70 to 69.70): BJ0

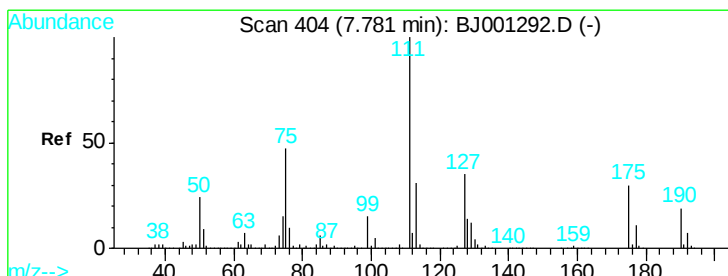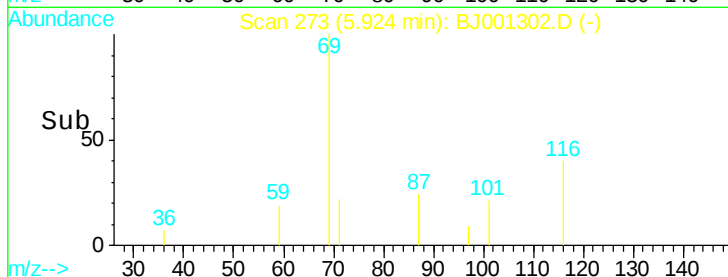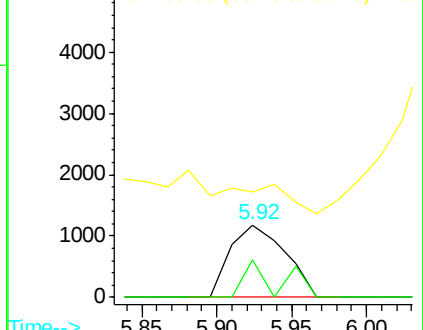

#14

p-Chlorophenylmethylsulfone

Concen: 0.02 ug/mL

RT: 7.74 min Scan# 401

Delta R.T. -0.04 min

Lab File: BJ001302.D

Acq: 27 Nov 2012 16:48

Tgt Ion:111 Resp: 4562


Ion Ratio Lower Upper

111 100

75 0.0 27.5 67.5#

127 0.0 15.3 55.3#

190 0.0 0.0 38.6

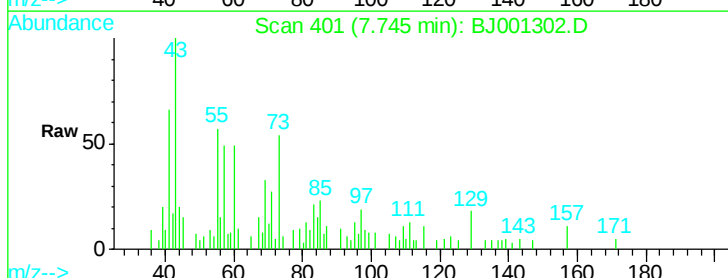

Abundance

Ion 111.00 (110.70 to 111.70): E

Ion 75.00 (74.70 to 75.70): BJ0

Ion 127.00 (126.70 to 127.70): E

Ion 190.00 (189.70 to 190.70): E

