

Data File : H:\VOL1\GCMSDATA\J\121127\BJ001305.D
 Acq On : 27 Nov 2012 17:40
 Sample : D4921-06
 Misc : WATER BNA J HLM
 MS Integration Params: rteint.p
 Quant Time: Nov 28 14:03 2012

Vial: 17
 Operator: HLM
 Inst : BNA J
 Multiplr: 1.00

Instrument :
 BNA_J
 ClientSampleId :
 CCDM164A-112012

Quant Results File: BJ112712.FRES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M (RTE Integrator)
 Title : CWA degradation products by GCMS
 Last Update : Tue Nov 27 14:50:43 2012
 Response via : Initial Calibration
 DataAcq Meth : CWAJ

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	152	301607	2.50	ug/mL	0.00
6) Naphthalene-d8	5.62	136	1245109	2.50	ug/mL	0.00
System Monitoring Compounds						
10) Tripropylphosphate	6.71	99	240084	0.48	ug/mL	0.00
Spiked Amount 0.500	Range	70 - 130	Recovery	=	96.00%	
12) 2-Bromothioanisole	6.92	204	343948	4.15	ug/mL	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	83.00%	
Target Compounds						
8) Thiodiglycol	5.55	61	2748	0.03	ug/mL#	1
14) p-Chlorophenylmethanesulfon	7.74	111	5914	0.03	ug/mL#	62

Data File : H:\VOL1\GCMSDATA\J\121127\BJ001305.D

Vial: 17

Acq On : 27 Nov 2012 17:40

Operator: HLM

Sample : D4921-06

Inst : BNA J

Misc : WATER BNA J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Nov 28 14:03 2012

Quant Results File: BJ112712.KES

Instrument :

BNA_J

ClientSampleId :


CCDM164A-112012


Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M (RTE Integrator)

Title : CWA degradation products by GCMS

Last Update : Tue Nov 27 14:50:43 2012

Response via : Initial Calibration

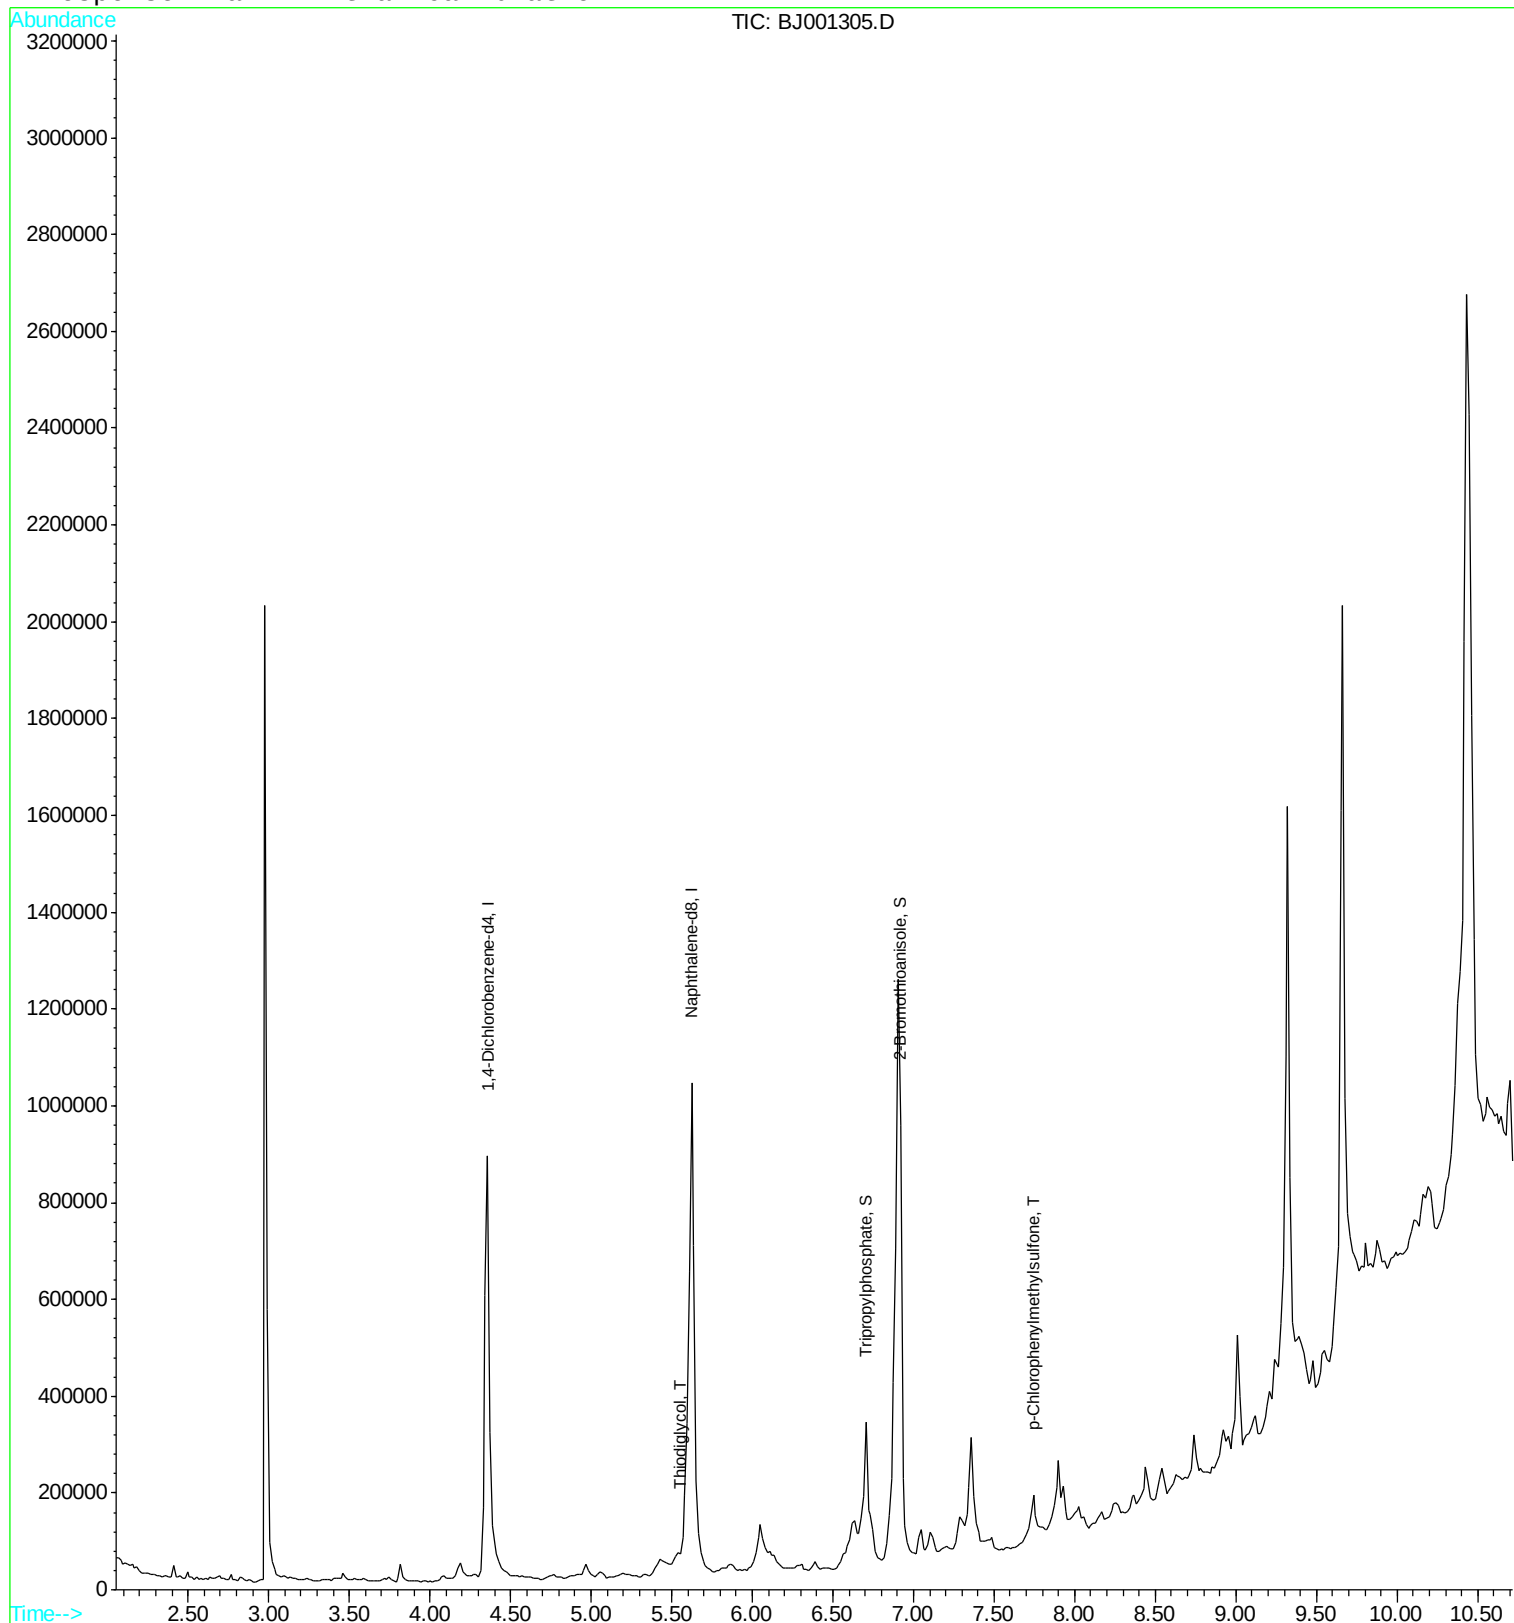

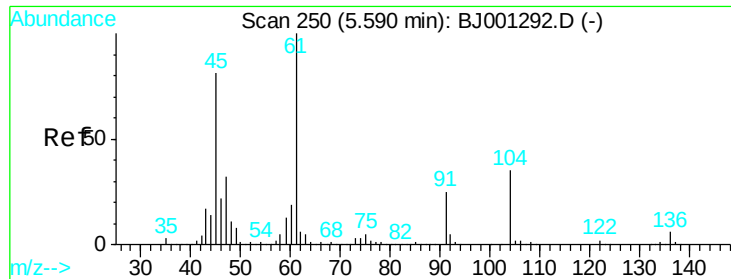

#8

Thiodiglycol

Concen: 0.03 ug/mL

RT: 5.55 min Scan# 247

Delta R.T. -0.04 min

Lab File: BJ001305.D

Acq: 27 Nov 2012 17:40

Instrument :

BNA_J

ClientSampleId :

CCDM164A-112012





Tgt Ion: 61 Resp: 2748

Ion Ratio Lower Upper

61 100

45 1180.0 61.0 101.0#

47 0.0 12.2 52.2#

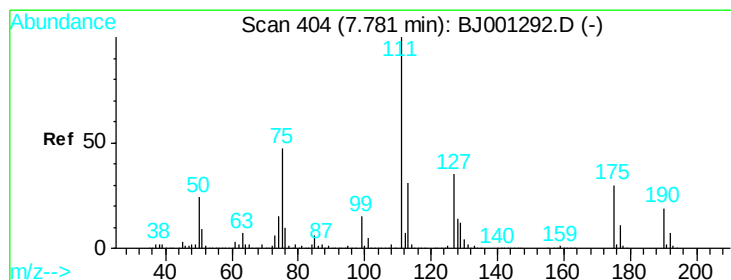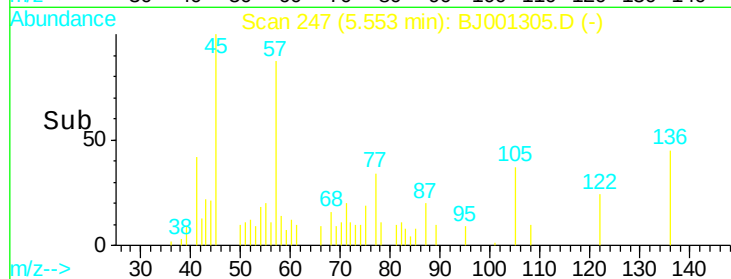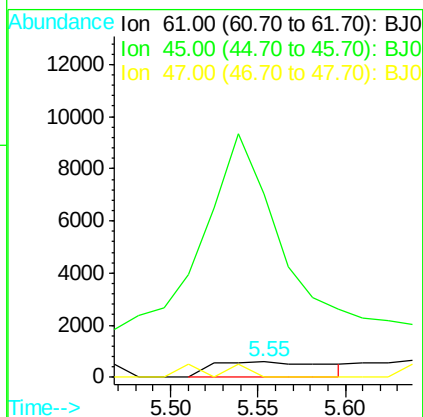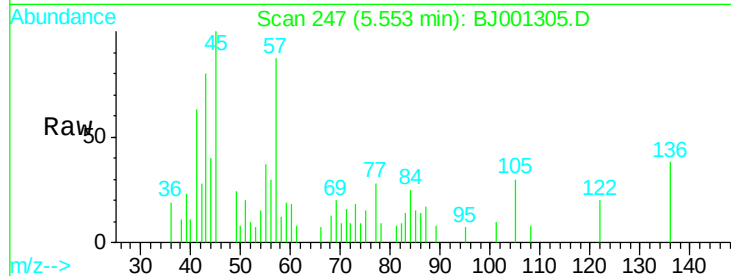

#14

p-Chlorophenylmethylsulfone

Concen: 0.03 ug/mL

RT: 7.74 min Scan# 401

Delta R.T. -0.04 min

Lab File: BJ001305.D

Acq: 27 Nov 2012 17:40

Tgt Ion: 111 Resp: 5914

Ion Ratio Lower Upper

111 100

75 33.7 27.5 67.5

127 0.0 15.3 55.3#

190 0.0 0.0 38.6

