

Data File : H:\VOL1\GCMSDATA\J\121127\BJ001306.D
 Acq On : 27 Nov 2012 17:57
 Sample : D4921-07
 Misc : WATER BNA J HLM
 MS Integration Params: rteint.p
 Quant Time: Nov 28 14:03 2012

Vial: 18
 Operator: HLM
 Inst : BNA J
 Multiplr: 1.00

Instrument :
 BNA_J
 ClientSampleId :
 CCDM163A-111912

Quant Results File: BJ112712.FRES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M (RTE Integrator)
 Title : CWA degradation products by GCMS
 Last Update : Tue Nov 27 14:50:43 2012
 Response via : Initial Calibration
 DataAcq Meth : CWAJ

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.35	152	262328	2.50	ug/mL	0.00
6) Naphthalene-d8	5.63	136	1112907	2.50	ug/mL	0.02
System Monitoring Compounds						
10) Tripropylphosphate	6.71	99	223470	0.50	ug/mL	0.02
Spiked Amount 0.500	Range	70 - 130	Recovery	=	100.00%	
12) 2-Bromothioanisole	6.91	204	318590	4.30	ug/mL	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	86.00%	
Target Compounds						
4) DIMP	4.68	97	7314	0.04	ug/mL#	1
14) p-Chlorophenylmethysulfon	7.75	111	13664	0.09	ug/mL#	73

Quantitation Report


Data File : H:\VOL1\GCMSDATA\J\121127\BJ001306.D
Acq On : 27 Nov 2012 17:57
Sample : D4921-07
Misc : WATER BNA J HLM
MS Integration Params: rteint.p
Quant Time: Nov 28 14:03 2012




Vial: 18
Operator: HLM
Inst : BNA J
Multiplr: 1.00

Instrument :
BNA_J
ClientSampleId :
CCDM163A-111912

Quant Results File: BJ112712.KES

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M (RTE Integrator)
Title : CWA degradation products by GCMS
Last Update : Tue Nov 27 14:50:43 2012
Response via : Initial Calibration

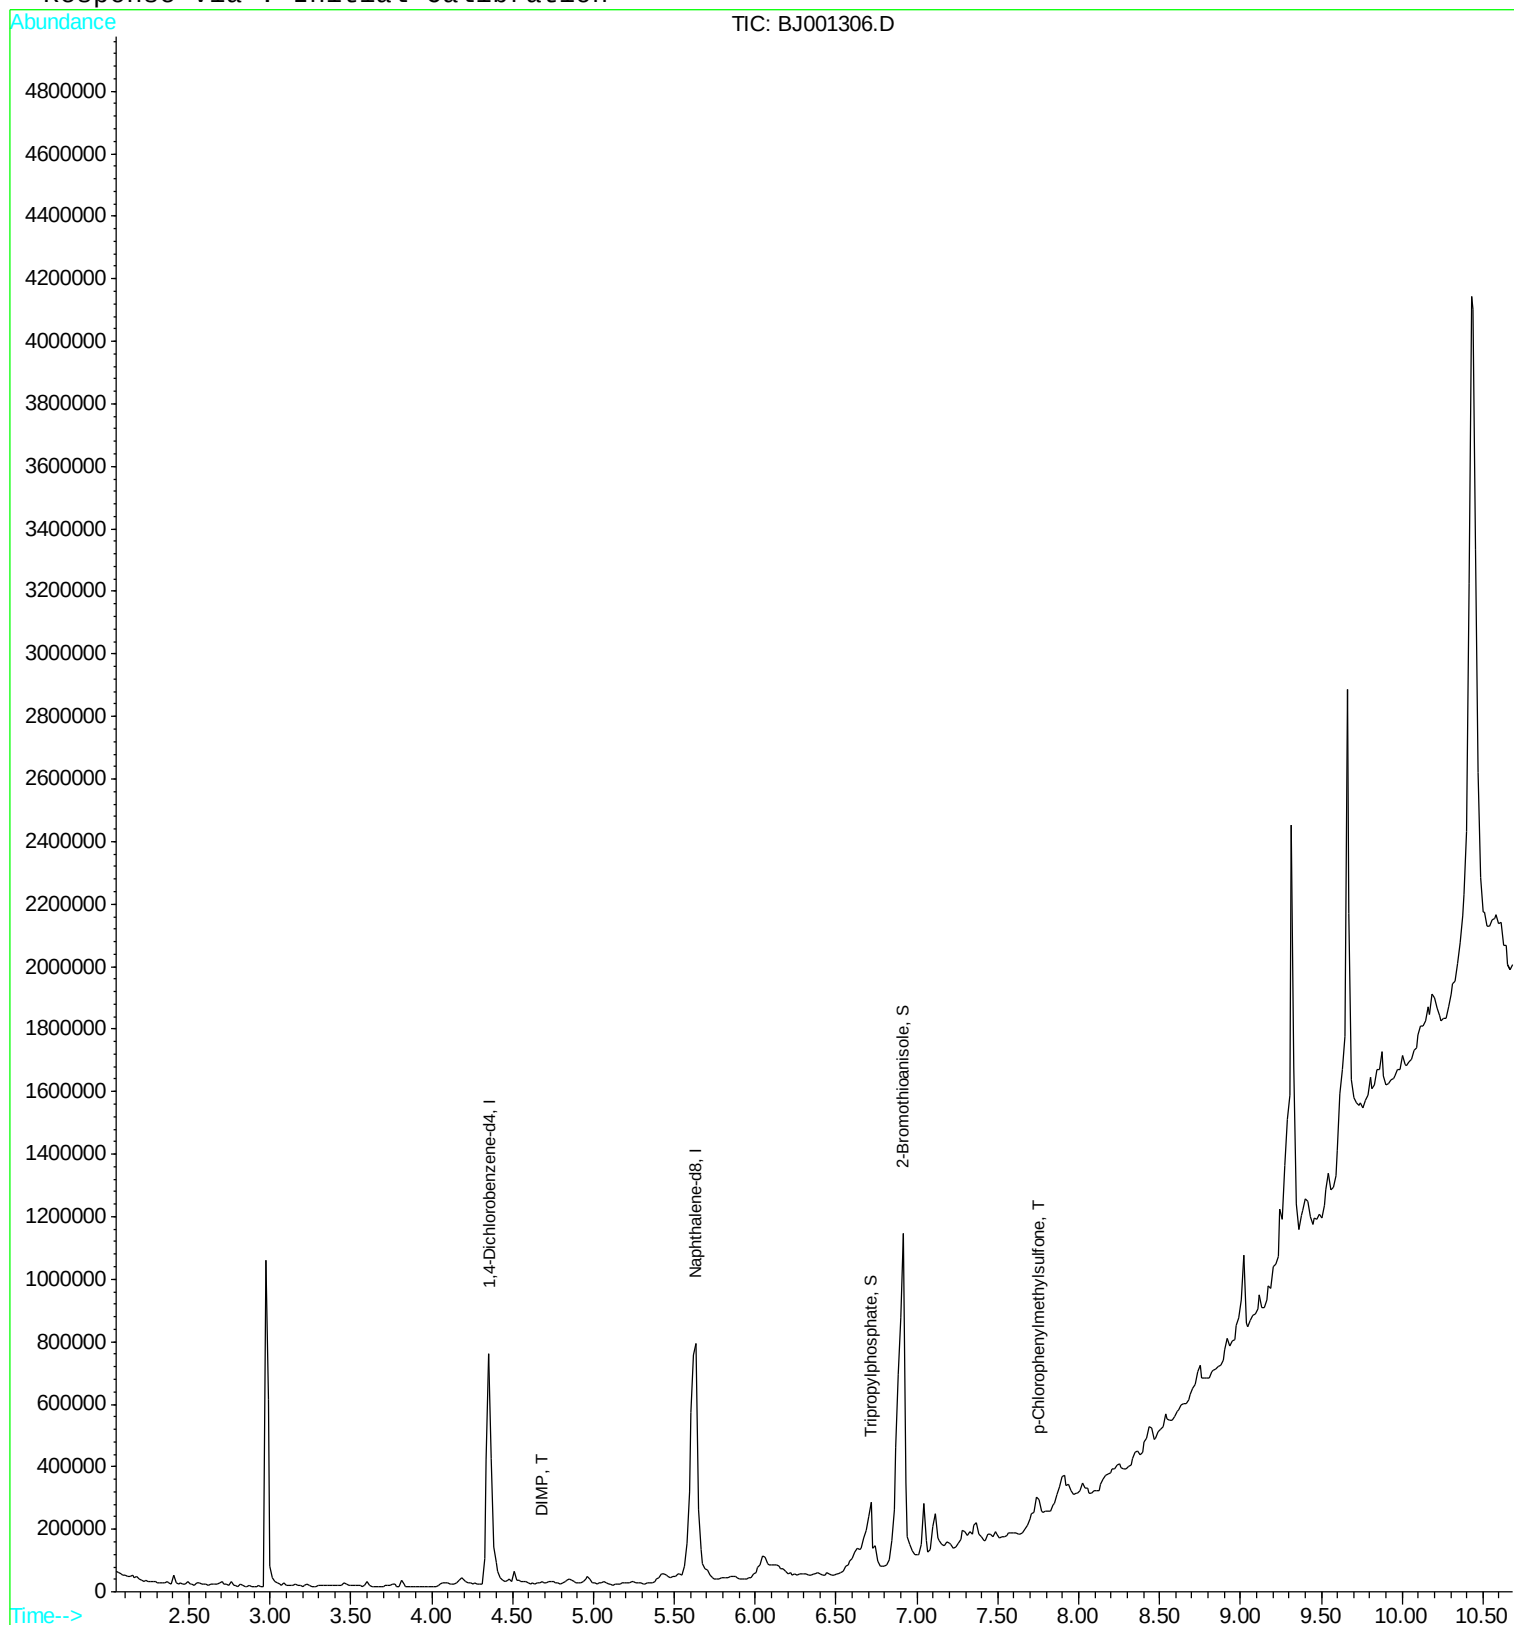

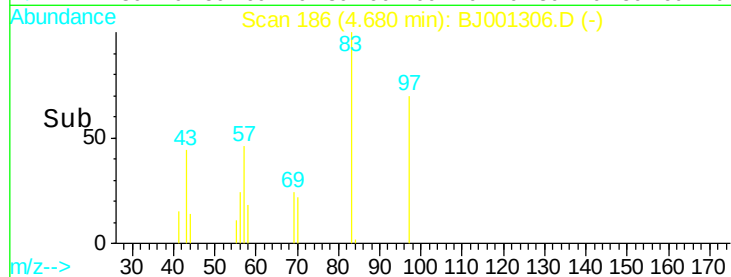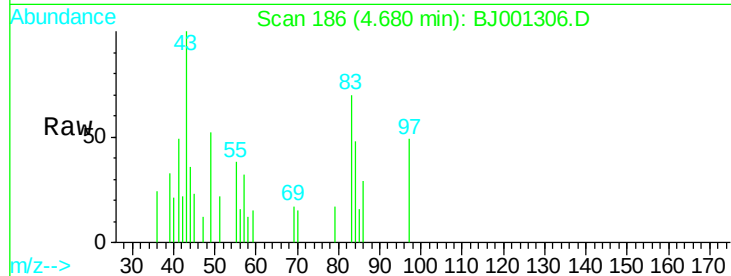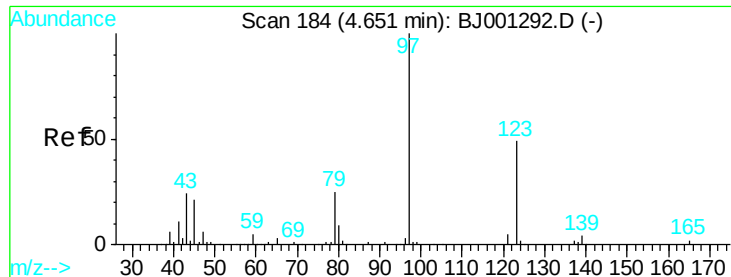

#4

DIMP

Concen: 0.04 ug/mL

RT: 4.68 min Scan# 186

Delta R.T. 0.03 min

Lab File: BJ001306.D

Acq: 27 Nov 2012 17:57

Instrument :

BNA_J

ClientSampleId :

CCDM163A-111912

Tgt Ion: 97 Resp: 7314





Ion Ratio Lower Upper

97 100

123 0.0 29.2 69.2#

43 205.6 4.0 44.0#

41 100.7 0.0 31.6#

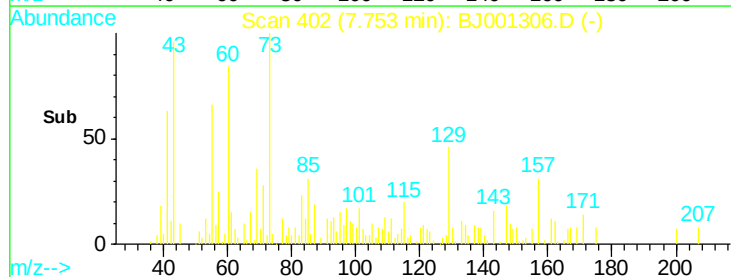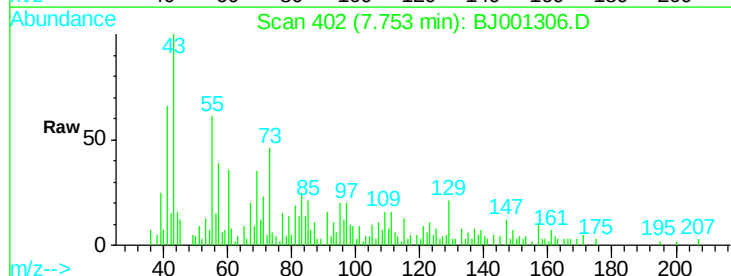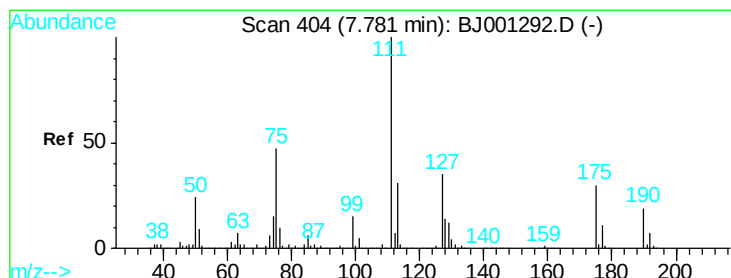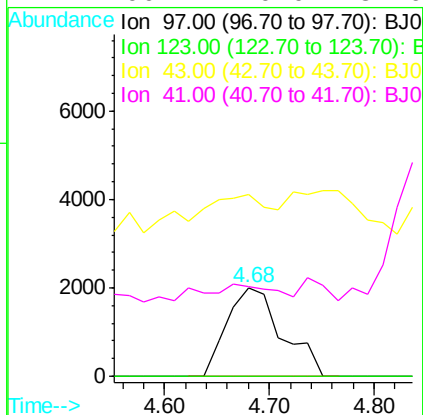

#14

p-Chlorophenylmethylsulfone

Concen: 0.09 ug/mL

RT: 7.75 min Scan# 402

Delta R.T. -0.03 min

Lab File: BJ001306.D

Acq: 27 Nov 2012 17:57

Tgt Ion:111 Resp: 13664

Ion Ratio Lower Upper

111 100

75 26.4 27.5 67.5#

127 26.9 15.3 55.3

190 0.0 0.0 38.6

