

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112712\
 Data File : BJ001303.D
 Acq On : 27 Nov 2012 17:05
 Operator : HLM
 Sample : D4921-04
 Misc : WATER BNA_J HLM
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 CC23A-112012R

Quant Time: Dec 05 03:16:42 2012
 Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M
 Quant Title : CWA degradation products by GCMS
 QLast Update : Tue Nov 27 14:50:43 2012
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	152	287769	2.50	ug/mL	0.00
6) Naphthalene-d8	5.62	136	1209482	2.50	ug/mL	0.00

System Monitoring Compounds						
10) Tripropylphosphate	6.70	99	239038	0.50	ug/mL	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.00%
12) 2-Bromothioanisole	6.92	204	331551	4.12	ug/mL	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%


Target Compounds						Qvalue
11) p-Chlorophenylmethanethiol	6.32	158	1634	0.01	ug/mL#	8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112712\
Data File : BJ001303.D
Acq On : 27 Nov 2012 17:05
Operator : HLM
Sample : D4921-04
Misc : WATER BNA_J HLM
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
CC23A-112012R

Quant Time: Dec 05 03:16:42 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M
Quant Title : CWA degradation products by GCMS
QLast Update : Tue Nov 27 14:50:43 2012
Response via : Initial Calibration

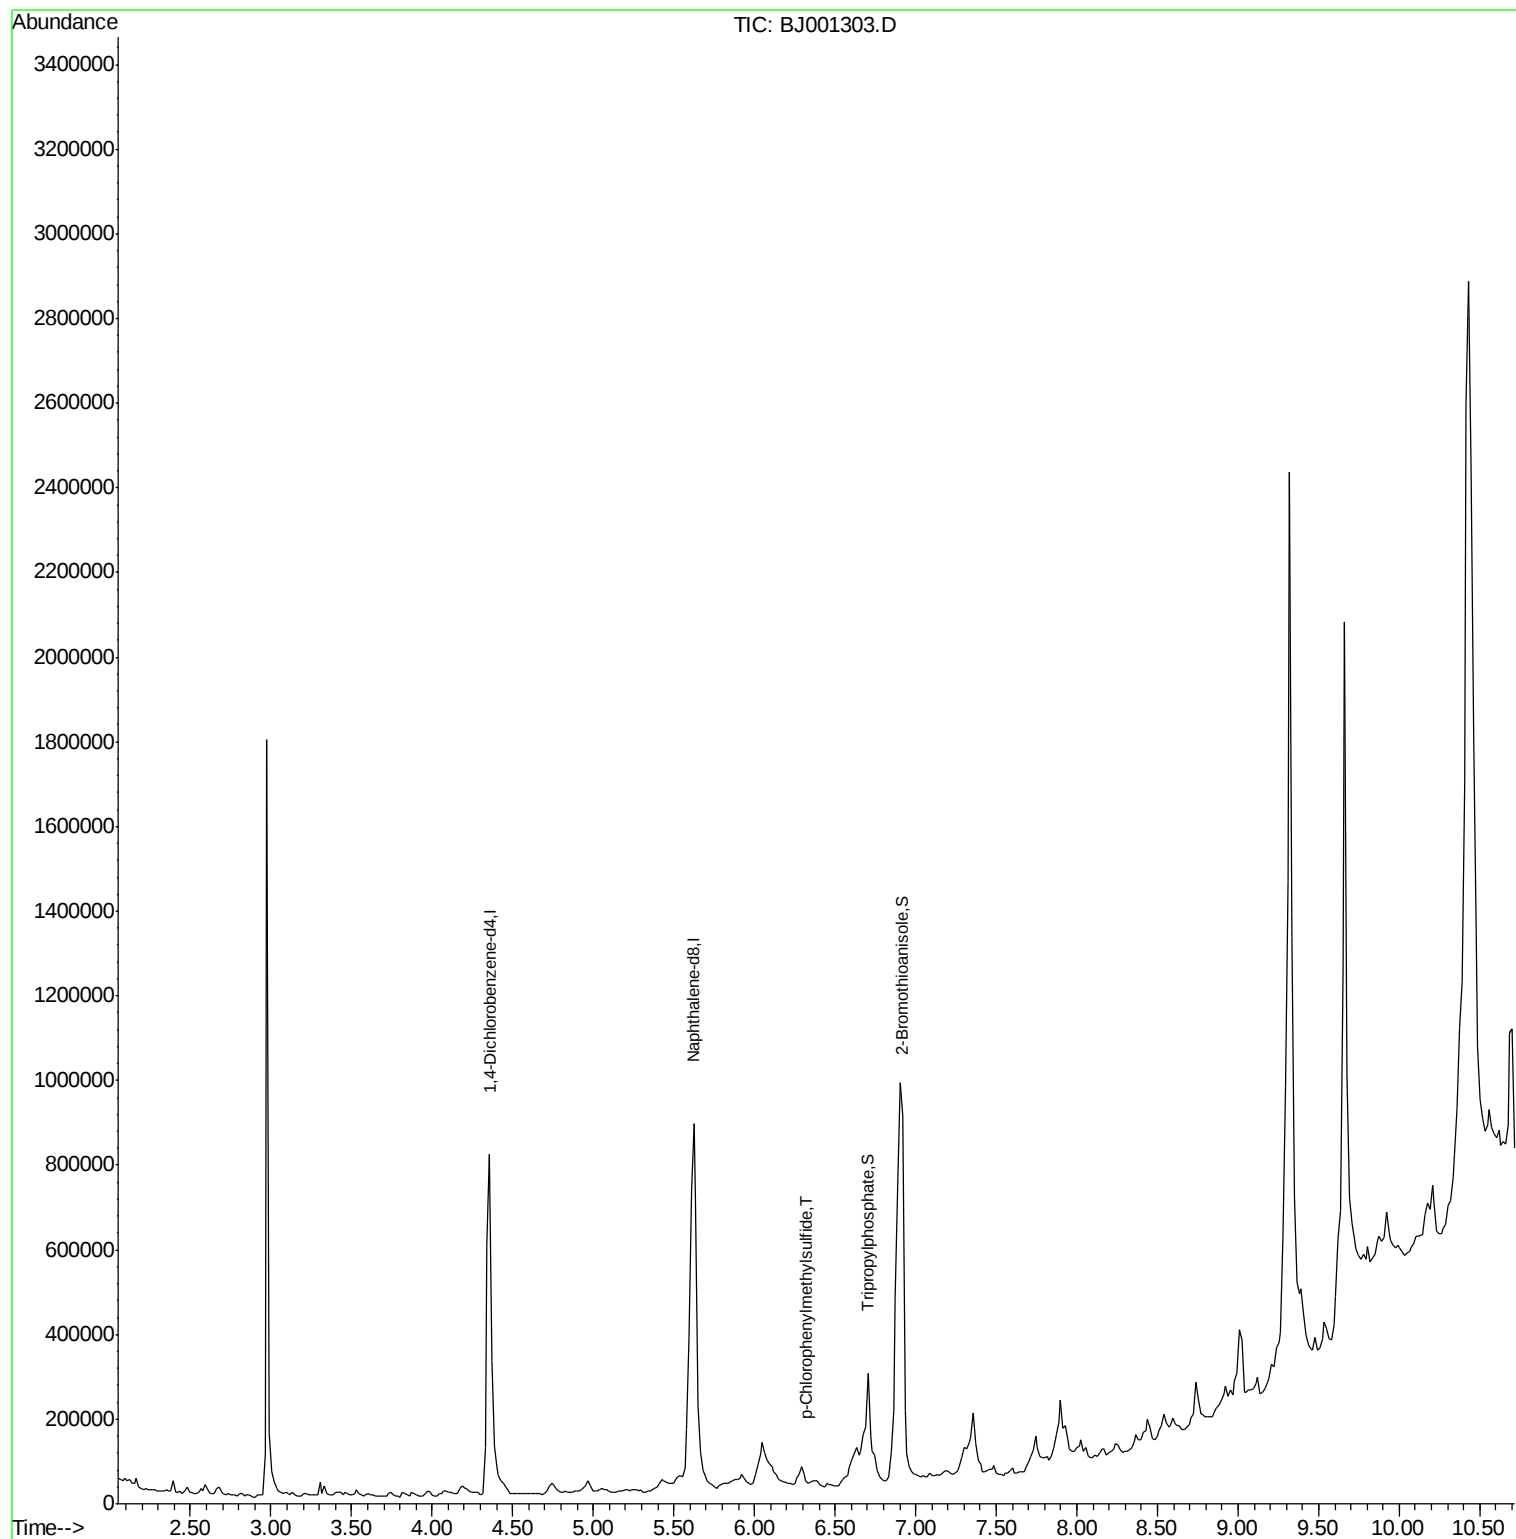

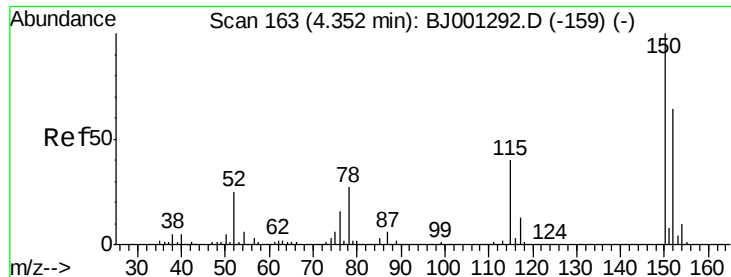


#1




1,4-Dichlorobenzene-d4
Concen: 2.50 ug/mL
RT: 4.36 min Scan# 163
Delta R.T. 0.00 min
Lab File: BJ001303.D
Acq: 27 Nov 2012 17:05

Instrument :
BNA_J
ClientSampleId :
CC23A-112012R

Tgt Ion:152 Resp: 287769
Ion Ratio Lower Upper
152 100
115 59.5 42.9 82.9

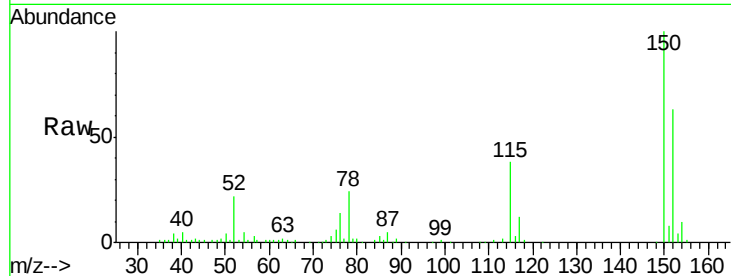


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 115.00 (114.70 to 115.70): E

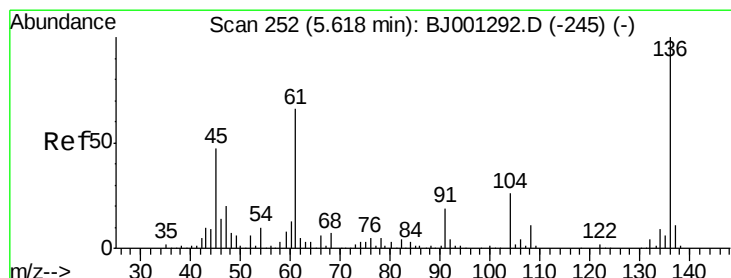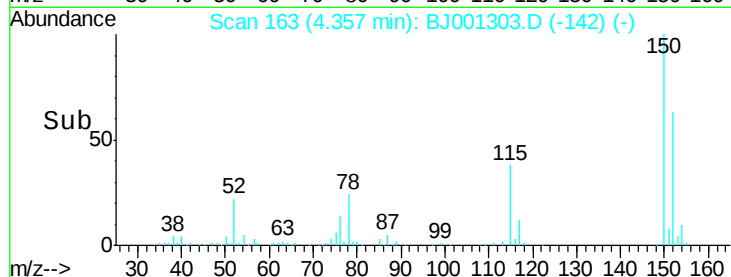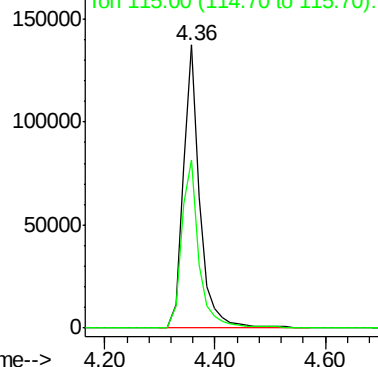



#6


Naphthalene-d8
Concen: 2.50 ug/mL
RT: 5.62 min Scan# 252
Delta R.T. 0.00 min
Lab File: BJ001303.D
Acq: 27 Nov 2012 17:05

Tgt Ion:136 Resp: 1209482
Ion Ratio Lower Upper
136 100
68 7.6 0.0 26.8

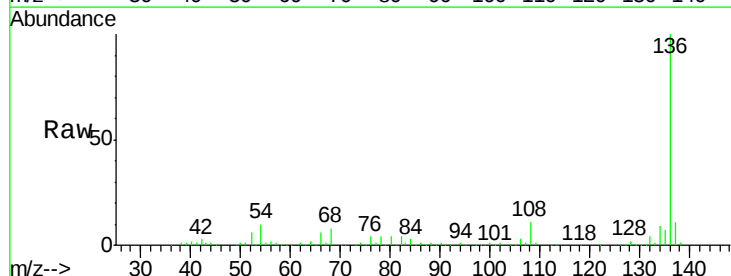

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 68.00 (67.70 to 68.70): BJ0

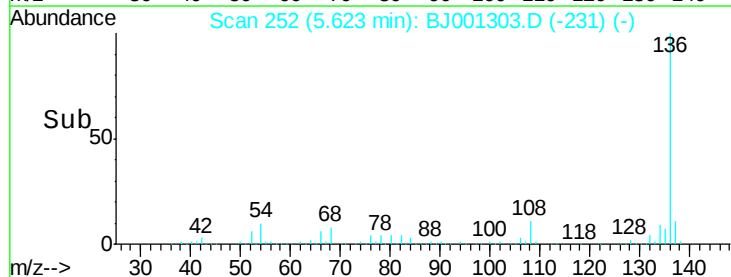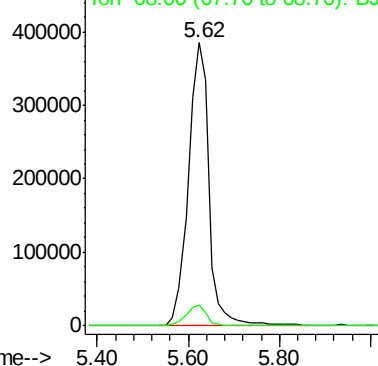

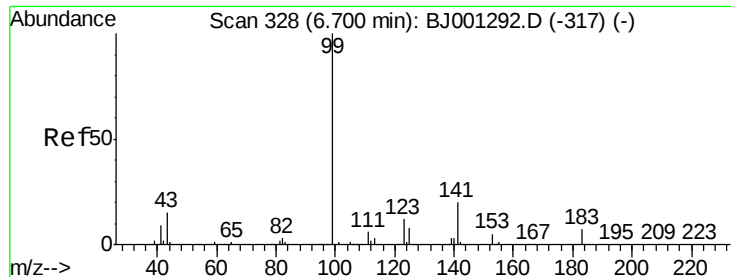

#10

Tripropylphosphate

Concen: 0.50 ug/mL

RT: 6.70 min Scan# 328

Delta R.T. 0.00 min

Lab File: BJ001303.D

Acq: 27 Nov 2012 17:05

Instrument :

BNA_J

ClientSampleId :

CC23A-112012R


Tgt Ion: 99 Resp: 239038

Ion Ratio Lower Upper

99 100

141 17.5 13.5 20.3




183 4.8 4.3 6.5

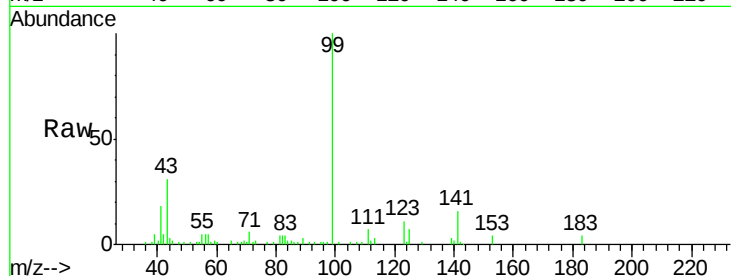

Abundance Ion 99.00 (98.70 to 99.70): BJ0

Ion 141.00 (140.70 to 141.70): BJ0

Ion 183.00 (182.70 to 183.70): BJ0

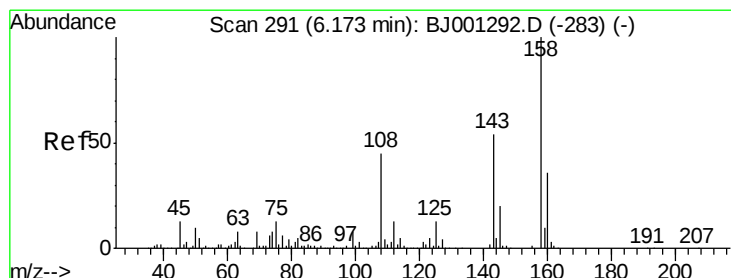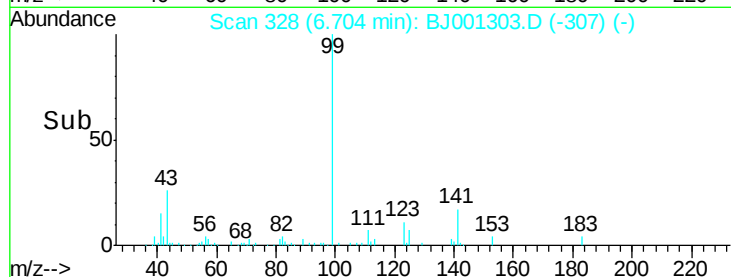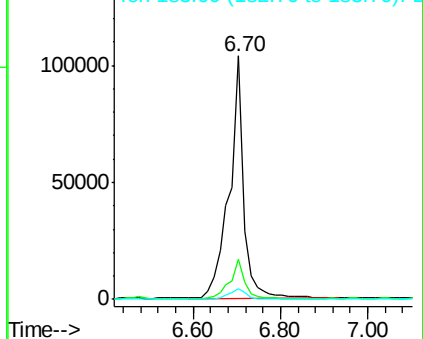

#11

p-Chlorophenylmethylsulfide

Concen: 0.01 ug/mL

RT: 6.32 min Scan# 301

Delta R.T. 0.15 min

Lab File: BJ001303.D

Acq: 27 Nov 2012 17:05

Tgt Ion: 158 Resp: 1634


Ion Ratio Lower Upper

158 100

143 0.0 34.4 74.4#

108 72.4 25.3 65.3#

45 141.3 0.0 34.7#


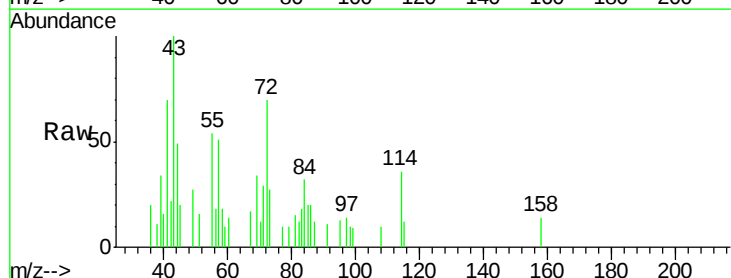



Abundance Ion 158.00 (157.70 to 158.70): BJ0

Ion 143.00 (142.70 to 143.70): BJ0

Ion 108.00 (107.70 to 108.70): BJ0

Ion 45.00 (44.70 to 45.70): BJ0

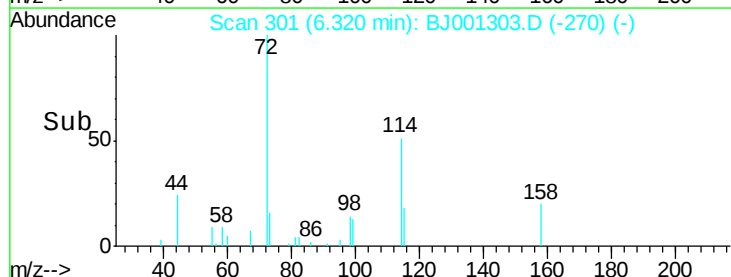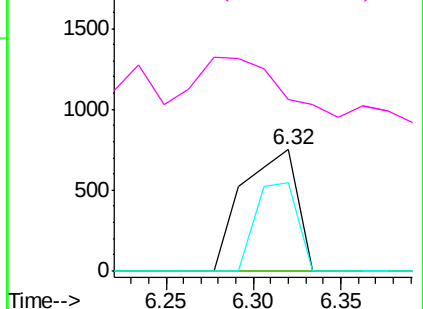


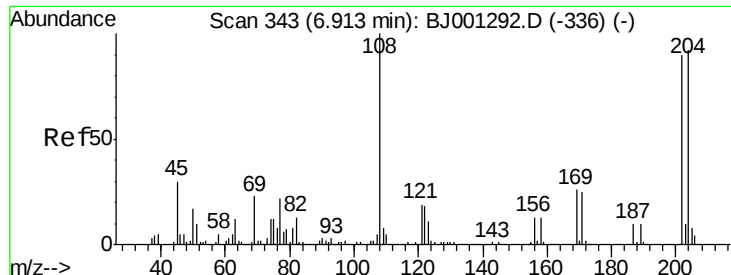

#12
 2-Bromothioanisole
 Concen: 4.12 ug/mL
 RT: 6.92 min Scan# 343
 Delta R.T. 0.00 min
 Lab File: BJ001303.D
 Acq: 27 Nov 2012 17:05

Instrument :
 BNA_J
 ClientSampleId :
 CC23A-112012R

Tgt Ion: 204 Resp: 331551
 Ion Ratio Lower Upper
 204 100
 202 98.3 77.8 117.8
 108 69.9 88.3 128.3#

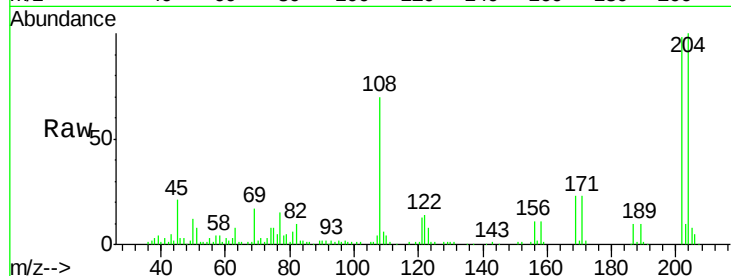

Abundance Ion 204.00 (203.70 to 204.70): E
 Ion 202.00 (201.70 to 202.70): E
 Ion 108.00 (107.70 to 108.70): E

