


Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ112712\
 Data File : BJ001289.D
 Acq On : 27 Nov 2012 12:14
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_J\METHOD\BJ112712.M
 Title : CWA degradation products by GCMS
 Last Update : Wed Nov 28 14:20:09 2012

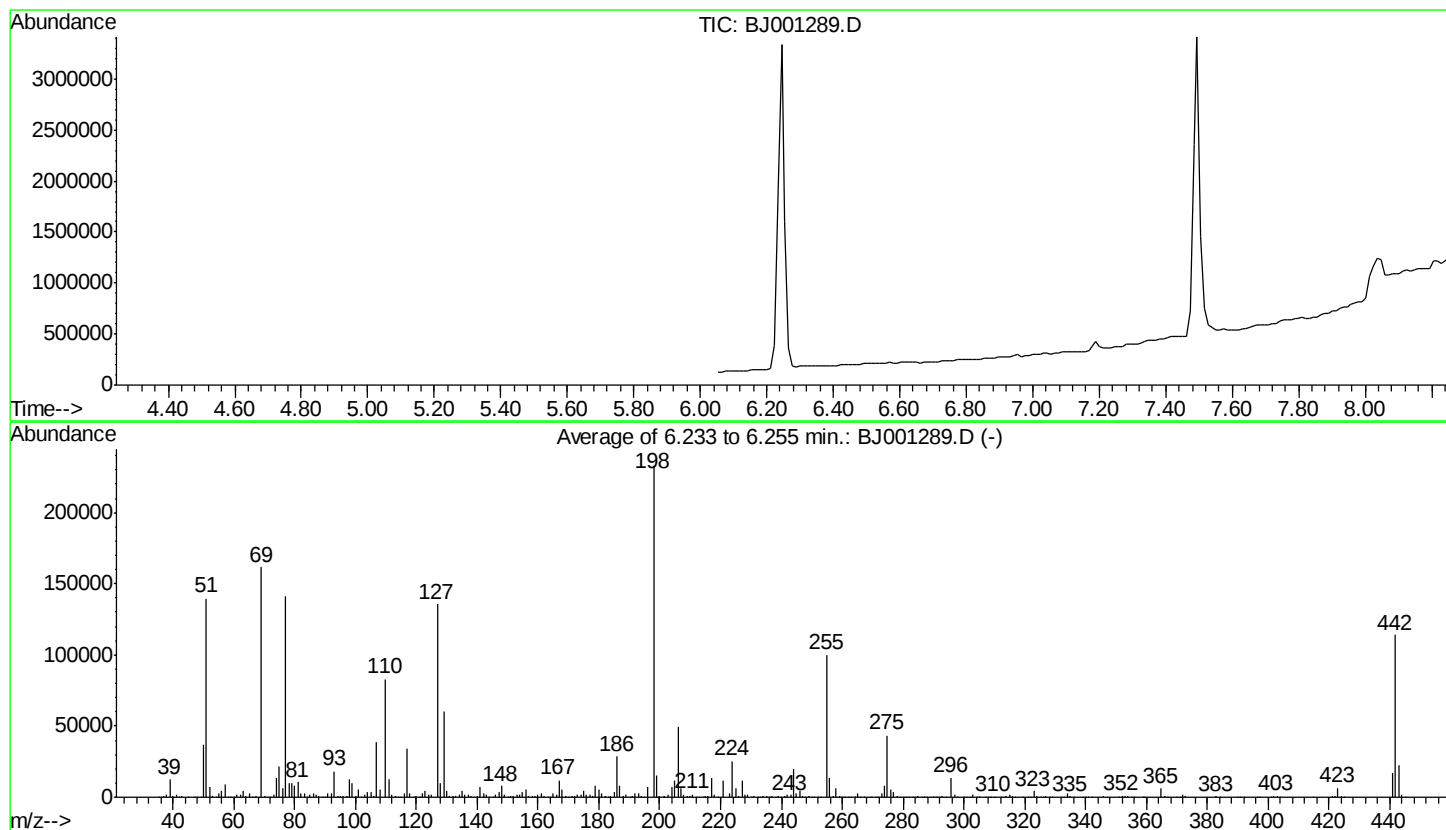

AutoFind: Scans 17, 18, 19; Background Corrected with Scan 9

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	60.0	139704	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	69.5	161821	PASS
70	69	0.00	2	0.5	822	PASS
127	198	40	60	58.2	135682	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	232960	PASS
199	198	5	9	6.7	15531	PASS
275	198	10	30	18.6	43242	PASS
365	198	1	100	2.6	6113	PASS
441	443	0.01	100	77.6	17122	PASS
442	198	40	100	49.0	114133	PASS
443	442	17	23	19.3	22067	PASS