

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ120412\
Data File : BJ001313.D
Acq On : 4 Dec 2012 17:06
Operator : HLM
Sample : PB67200BL
Misc : WATER BNA_J HLM
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB67200BL

Quant Time: Dec 08 04:28:29 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M
Quant Title : CWA degradation products by GCMS
QLast Update : Wed Dec 05 11:26:13 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	152	235640	2.00	ug/mL	-0.01
6) Naphthalene-d8	5.64	136	967647	2.00	ug/mL	0.00

System Monitoring Compounds

10) Tripropylphosphate	6.70	99	183973	0.38	ug/mL	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	76.00%
12) 2-Bromothioanisole	6.92	204	372246	4.62	ug/mL	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ120412\
Data File : BJ001313.D
Acq On : 4 Dec 2012 17:06
Operator : HLM
Sample : PB67200BL
Misc : WATER BNA_J HLM
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
PB67200BL

Quant Time: Dec 08 04:28:29 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M
Quant Title : CWA degradation products by GCMS
QLast Update : Wed Dec 05 11:26:13 2012
Response via : Initial Calibration

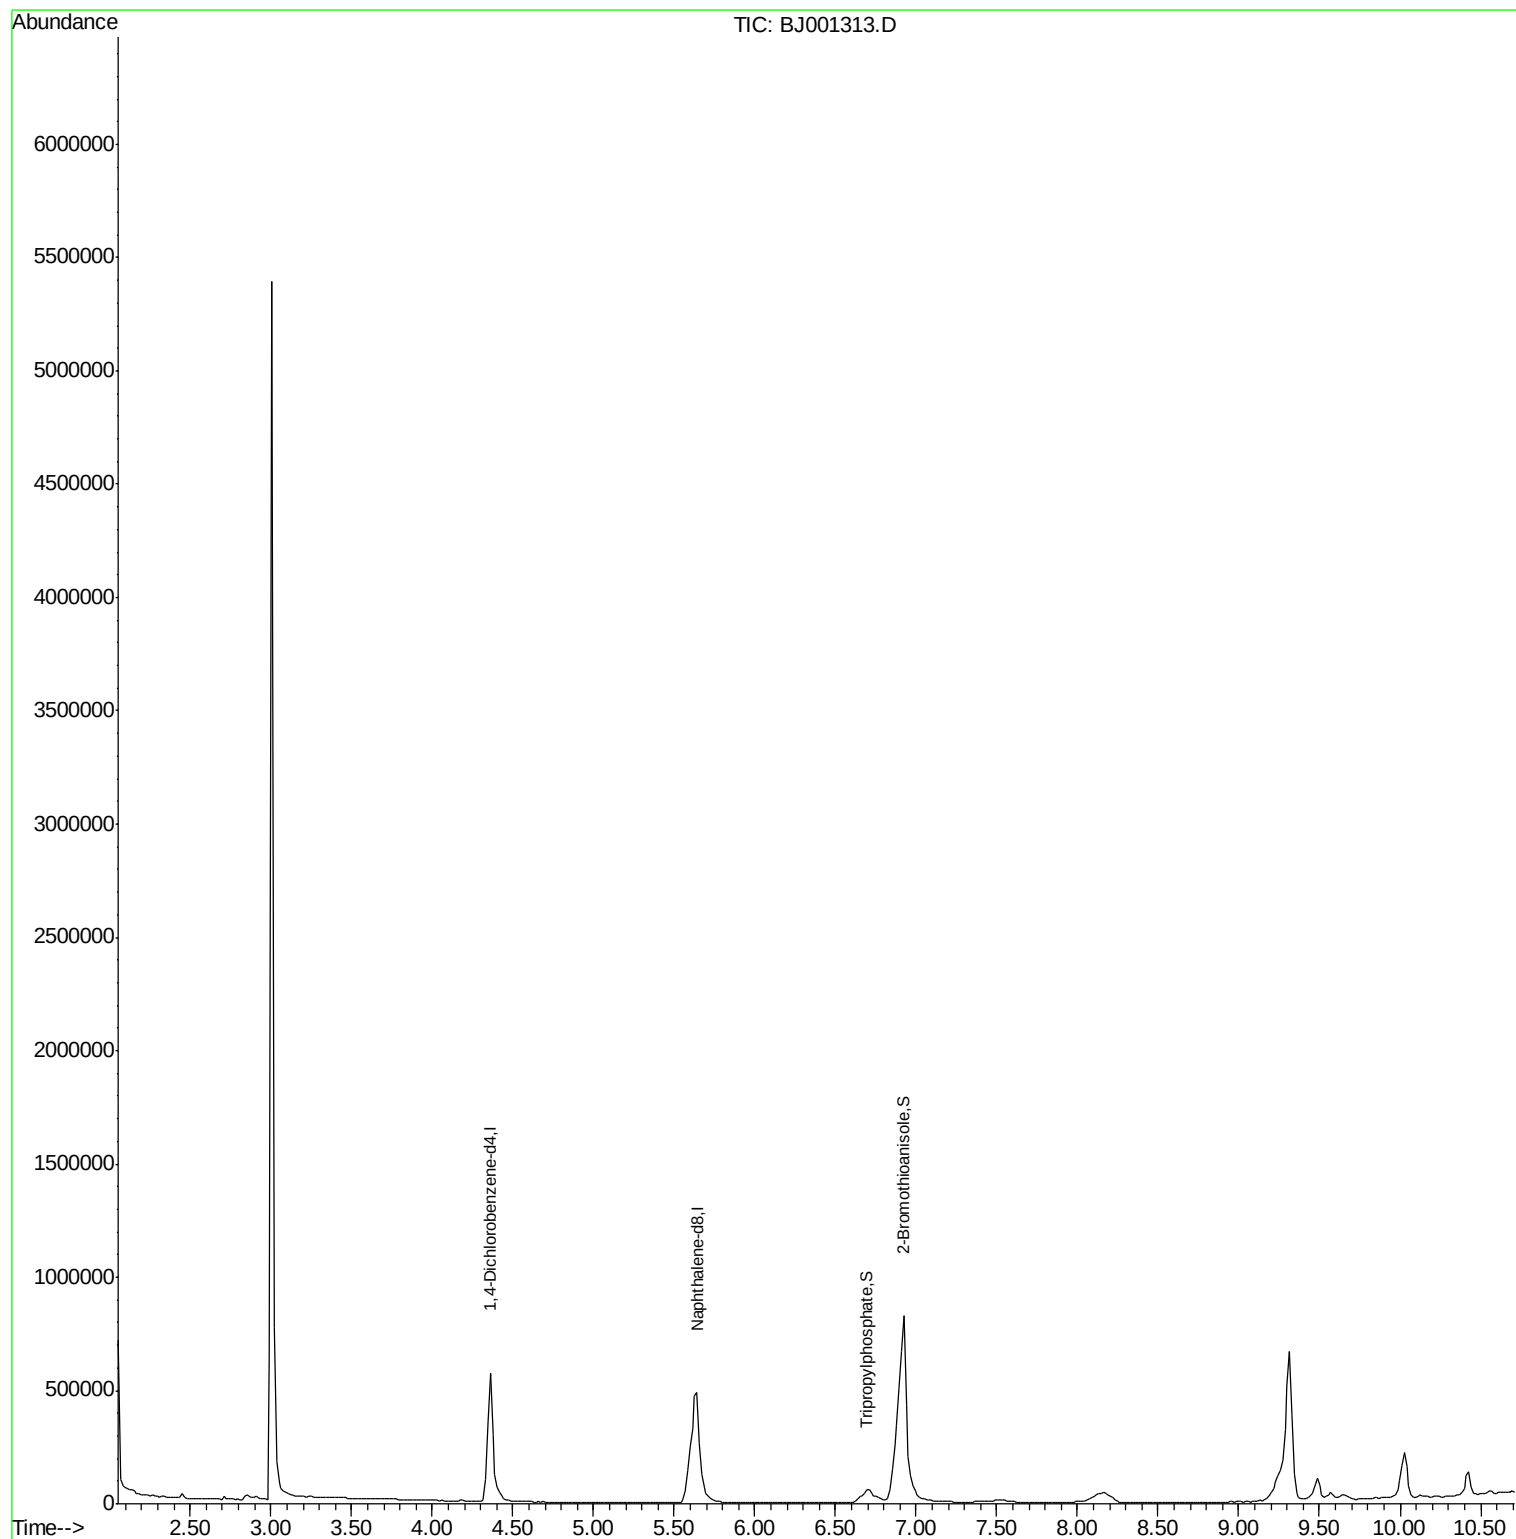

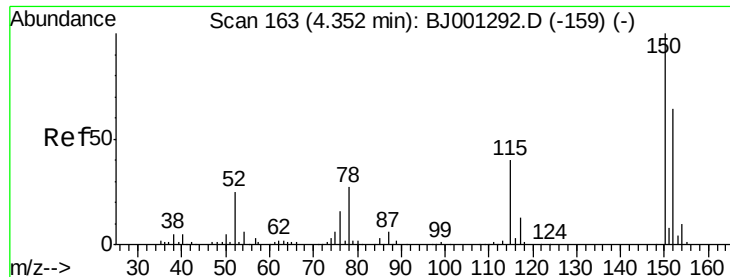


#1




1,4-Dichlorobenzene-d4
Concen: 2.00 ug/mL
RT: 4.36 min Scan# 163
Delta R.T. -0.01 min
Lab File: BJ001313.D
Acq: 4 Dec 2012 17:06

Instrument :
BNA_J
ClientSampleId :
PB67200BL

Tgt Ion:152 Resp: 235640
Ion Ratio Lower Upper
152 100
115 58.4 26.3 66.3

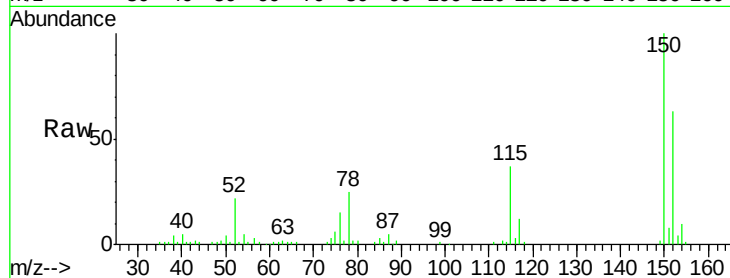


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 115.00 (114.70 to 115.70): E

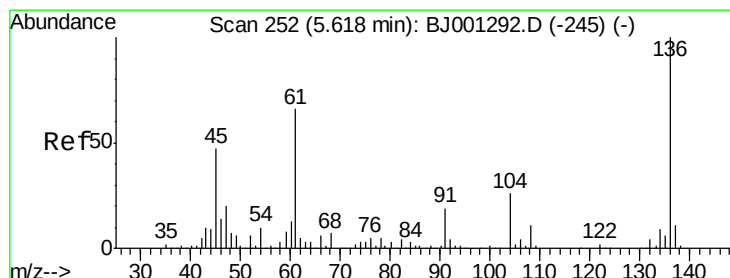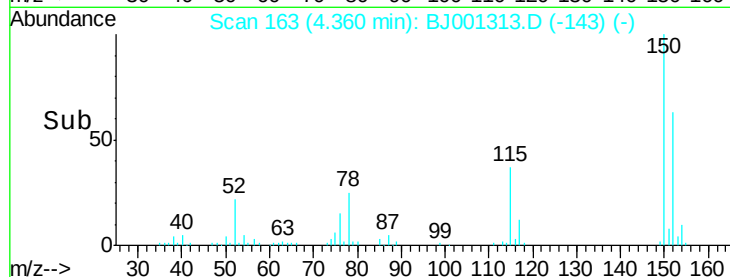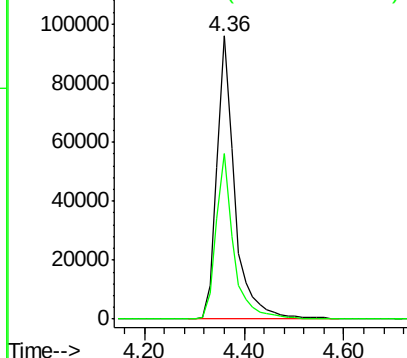



#6


Naphthalene-d8
Concen: 2.00 ug/mL
RT: 5.64 min Scan# 253
Delta R.T. 0.00 min
Lab File: BJ001313.D
Acq: 4 Dec 2012 17:06

Tgt Ion:136 Resp: 967647
Ion Ratio Lower Upper
136 100
68 7.7 0.0 25.9

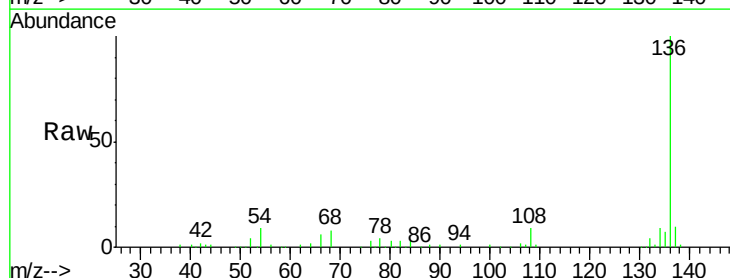

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 68.00 (67.70 to 68.70): BJ0

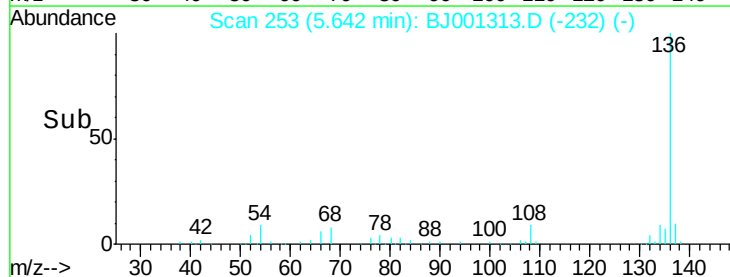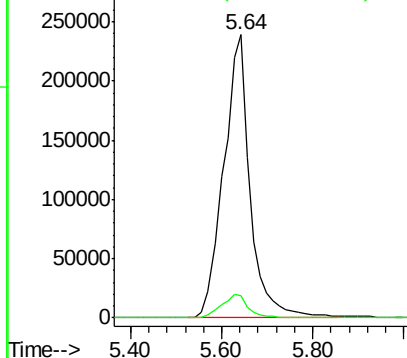

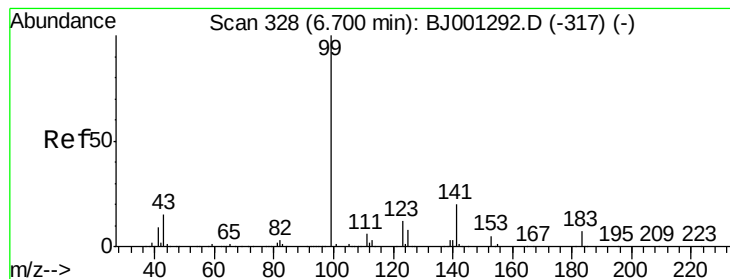

#10

Tripropylphosphate

Concen: 0.38 ug/mL

RT: 6.70 min Scan# 327

Delta R.T. 0.00 min

Lab File: BJ001313.D

Acq: 4 Dec 2012 17:06

Instrument :

BNA_J

ClientSampleId :

PB67200BL


Tgt Ion: 99 Resp: 183973

Ion Ratio Lower Upper

99 100

141 18.9 14.7 22.1




183 3.9 4.6 6.8#

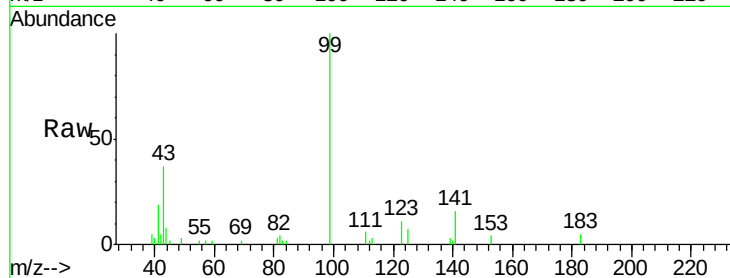

Abundance Ion 99.00 (98.70 to 99.70): BJ0

Ion 141.00 (140.70 to 141.70): E

Ion 183.00 (182.70 to 183.70): E

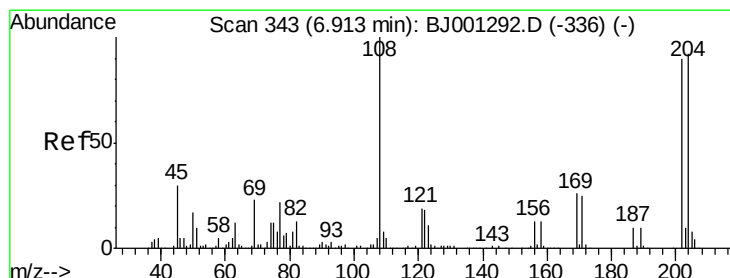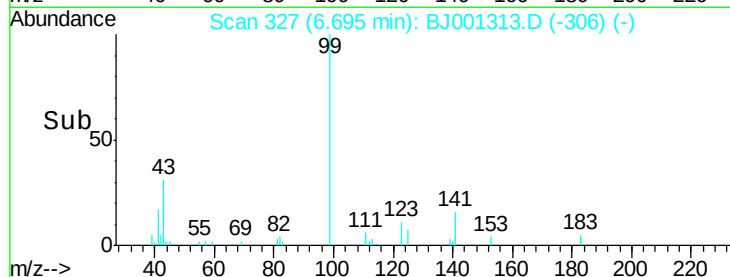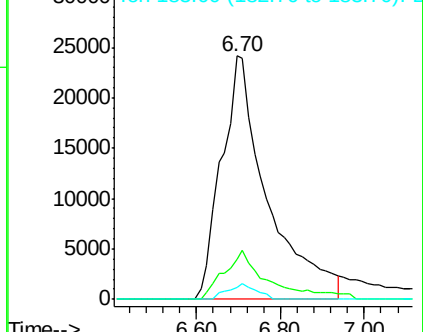

#12

2-Bromothioanisole

Concen: 4.62 ug/mL

RT: 6.92 min Scan# 343

Delta R.T. 0.00 min

Lab File: BJ001313.D

Acq: 4 Dec 2012 17:06


Tgt Ion: 204 Resp: 372246

Ion Ratio Lower Upper

204 100

202 100.6 80.7 120.7

108 100.6 87.3 127.3

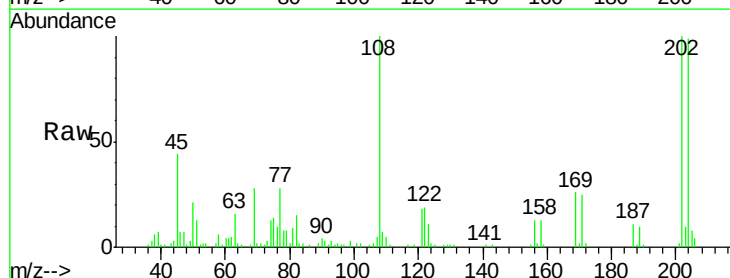

Abundance Ion 204.00 (203.70 to 204.70): E

Ion 202.00 (201.70 to 202.70): E

Ion 108.00 (107.70 to 108.70): E

