

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ120412\
Data File : BJ001317.D
Acq On : 4 Dec 2012 18:16
Operator : HLM
Sample : D4972-02
Misc : WATER BNA_J HLM
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
NMB65A-112812

Quant Time: Dec 08 04:30:13 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M
Quant Title : CWA degradation products by GCMS
QLast Update : Wed Dec 05 11:26:13 2012
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.36	152	238601	2.00	ug/mL	-0.02
6) Naphthalene-d8	5.64	136	989126	2.00	ug/mL	0.00

System Monitoring Compounds

10) Tripropylphosphate	6.71	99	280661	0.57	ug/mL	0.01
Spiked Amount	0.500	Range	70 - 130	Recovery	=	114.00%
12) 2-Bromothioanisole	6.92	204	430339	5.23	ug/mL	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ120412\
Data File : BJ001317.D
Acq On : 4 Dec 2012 18:16
Operator : HLM
Sample : D4972-02
Misc : WATER BNA_J HLM
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_J
ClientSampleId :
NMB65A-112812

Quant Time: Dec 08 04:30:13 2012
Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ112712.M
Quant Title : CWA degradation products by GCMS
QLast Update : Wed Dec 05 11:26:13 2012
Response via : Initial Calibration

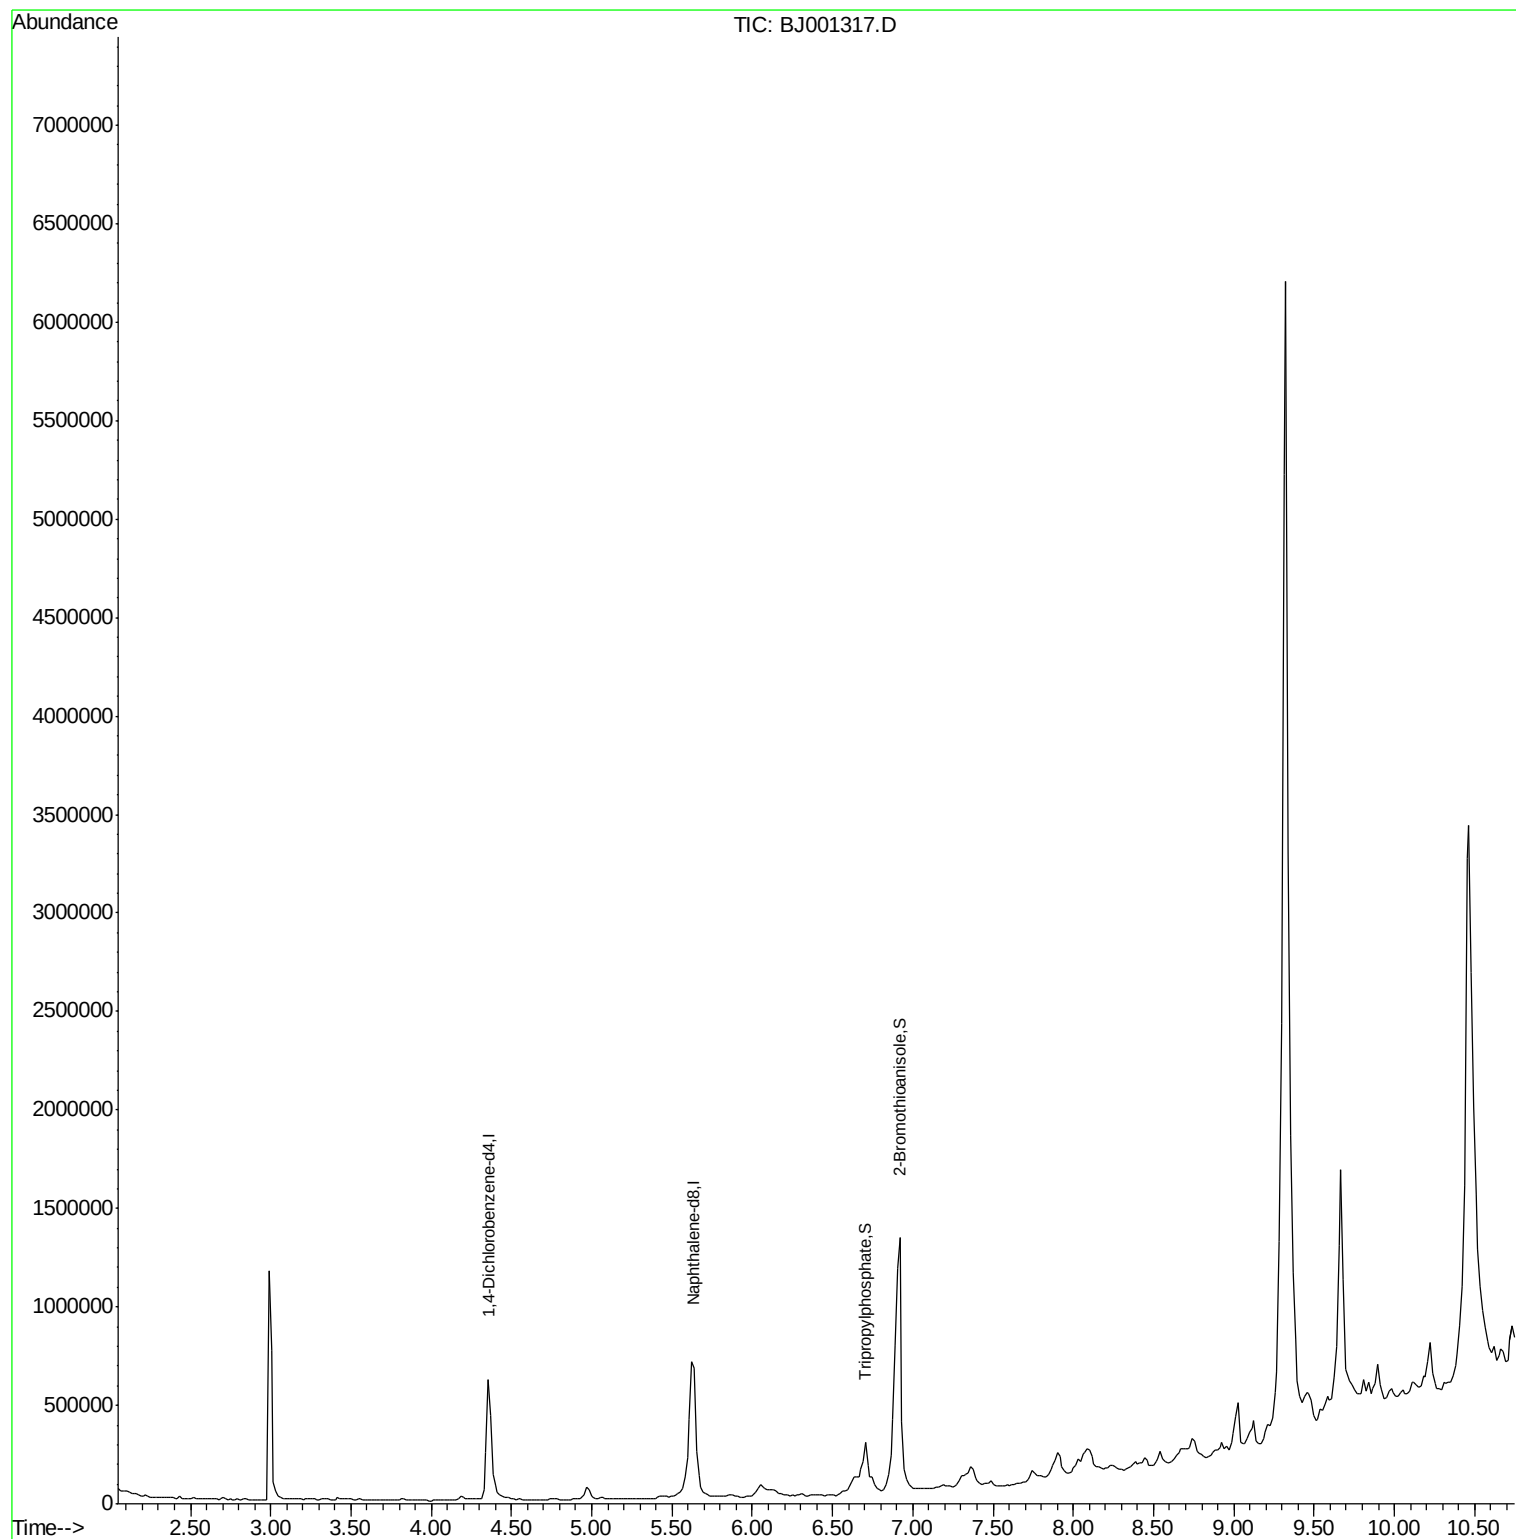

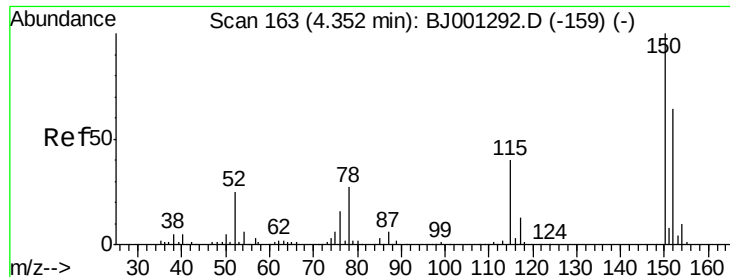


#1




1,4-Dichlorobenzene-d4
 Concen: 2.00 ug/mL
 RT: 4.36 min Scan# 163
 Delta R.T. -0.02 min
 Lab File: BJ001317.D
 Acq: 4 Dec 2012 18:16

Instrument :
 BNA_J
 ClientSampleId :
 NMB65A-112812

Tgt Ion:152 Resp: 238601
 Ion Ratio Lower Upper
 152 100
 115 61.6 26.3 66.3

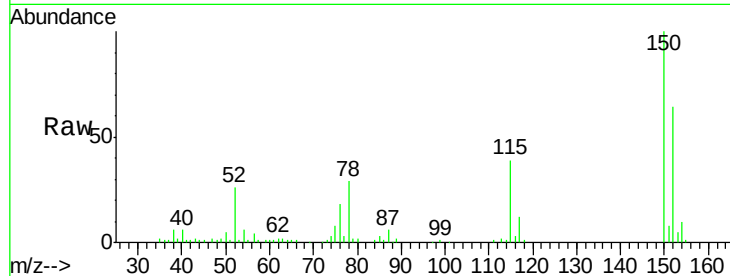


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 115.00 (114.70 to 115.70): E

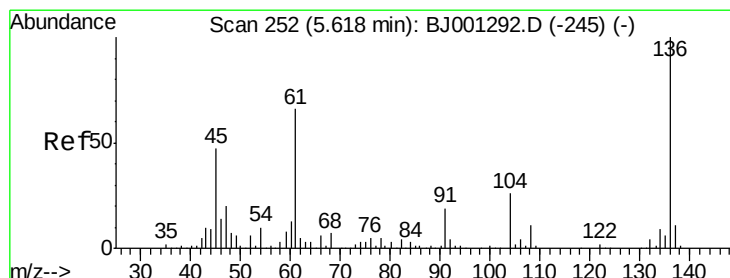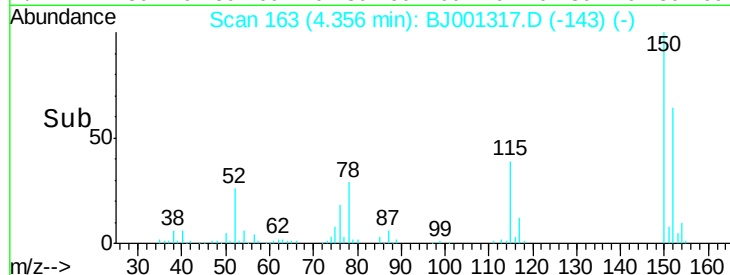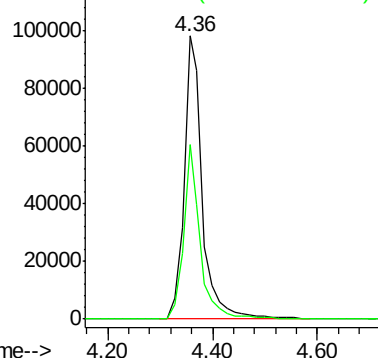



#6


Naphthalene-d8
 Concen: 2.00 ug/mL
 RT: 5.64 min Scan# 253
 Delta R.T. -0.00 min
 Lab File: BJ001317.D
 Acq: 4 Dec 2012 18:16

Tgt Ion:136 Resp: 989126
 Ion Ratio Lower Upper
 136 100
 68 7.1 0.0 25.9

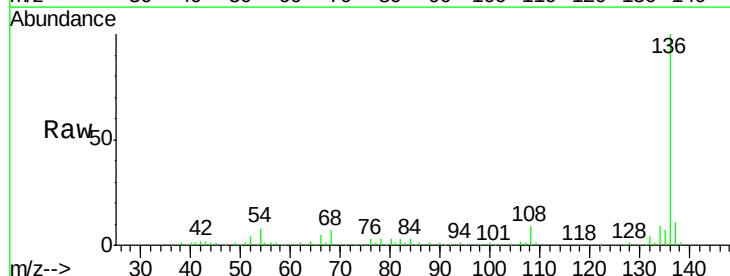

Abundance Ion 136.00 (135.70 to 136.70): E
 Ion 68.00 (67.70 to 68.70): BJ0

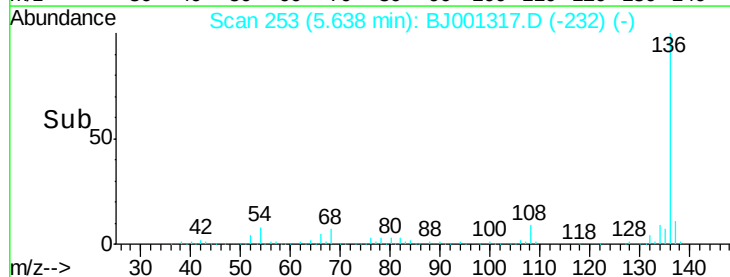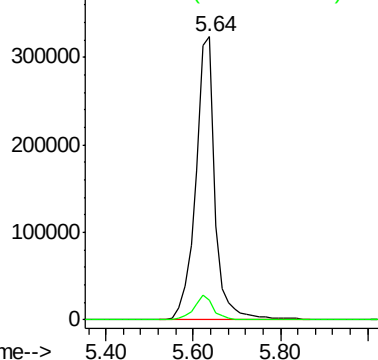

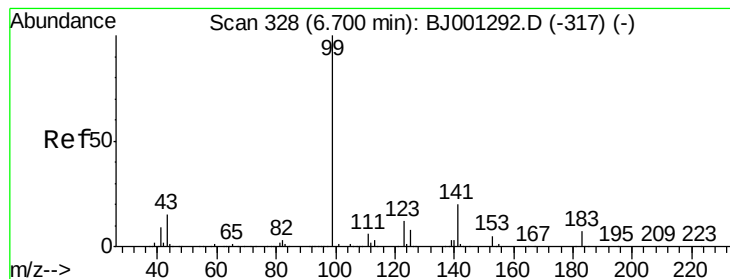

#10

Tripropylphosphate

Concen: 0.57 ug/mL

RT: 6.71 min Scan# 328

Delta R.T. 0.01 min

Lab File: BJ001317.D

Acq: 4 Dec 2012 18:16

Instrument :

BNA_J

ClientSampleId :

NMB65A-112812


Tgt Ion: 99 Resp: 280661

Ion Ratio Lower Upper

99 100

141 17.2 14.7 22.1




183 4.9 4.6 6.8

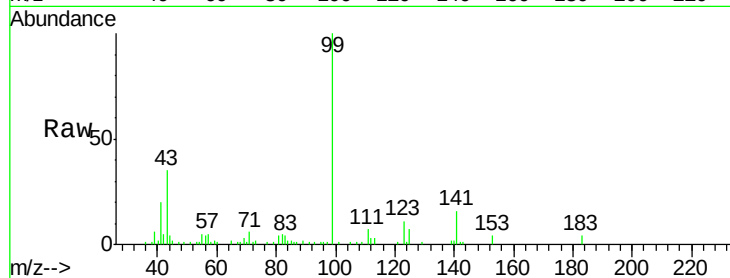

Abundance Ion 99.00 (98.70 to 99.70): BJ0

Ion 141.00 (140.70 to 141.70): E

Ion 183.00 (182.70 to 183.70): E

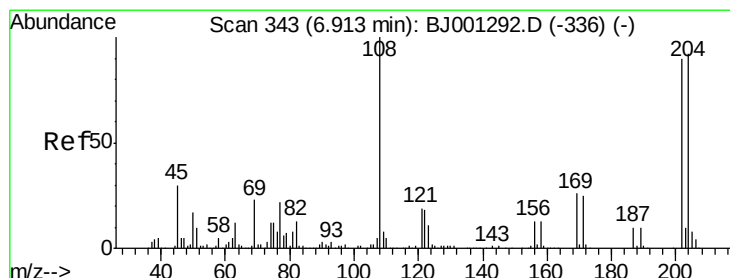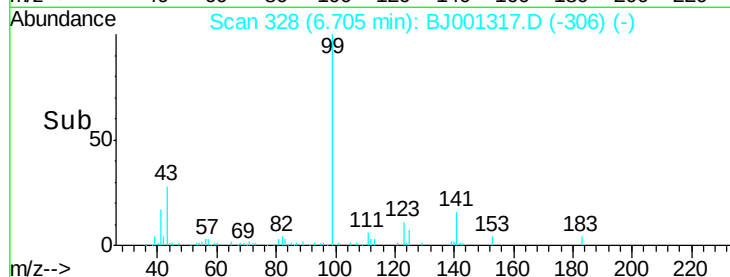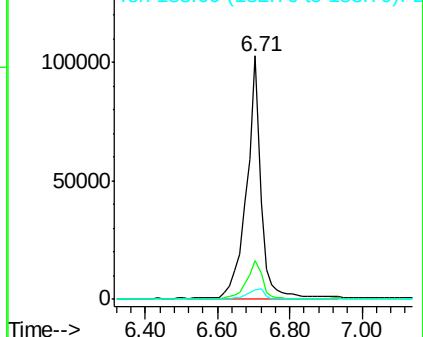

#12

2-Bromothioanisole

Concen: 5.23 ug/mL

RT: 6.92 min Scan# 343

Delta R.T. -0.00 min

Lab File: BJ001317.D

Acq: 4 Dec 2012 18:16


Tgt Ion: 204 Resp: 430339

Ion Ratio Lower Upper

204 100

202 98.8 80.7 120.7

108 94.0 87.3 127.3

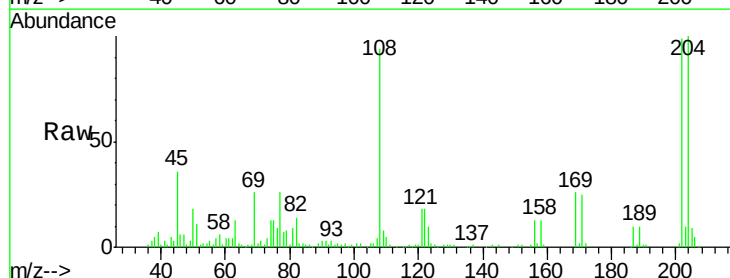

Abundance Ion 204.00 (203.70 to 204.70): E

Ion 202.00 (201.70 to 202.70): E

Ion 108.00 (107.70 to 108.70): E

