


Data Path : Z:\HPCHEM1\BNA_J\DATA\BJ120412\
 Data File : BJ001311.D
 Acq On : 4 Dec 2012 15:52
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_J\METHOD\BJ112712.M
 Title : CWA degradation products by GCMS
 Last Update : Wed Nov 28 14:20:09 2012

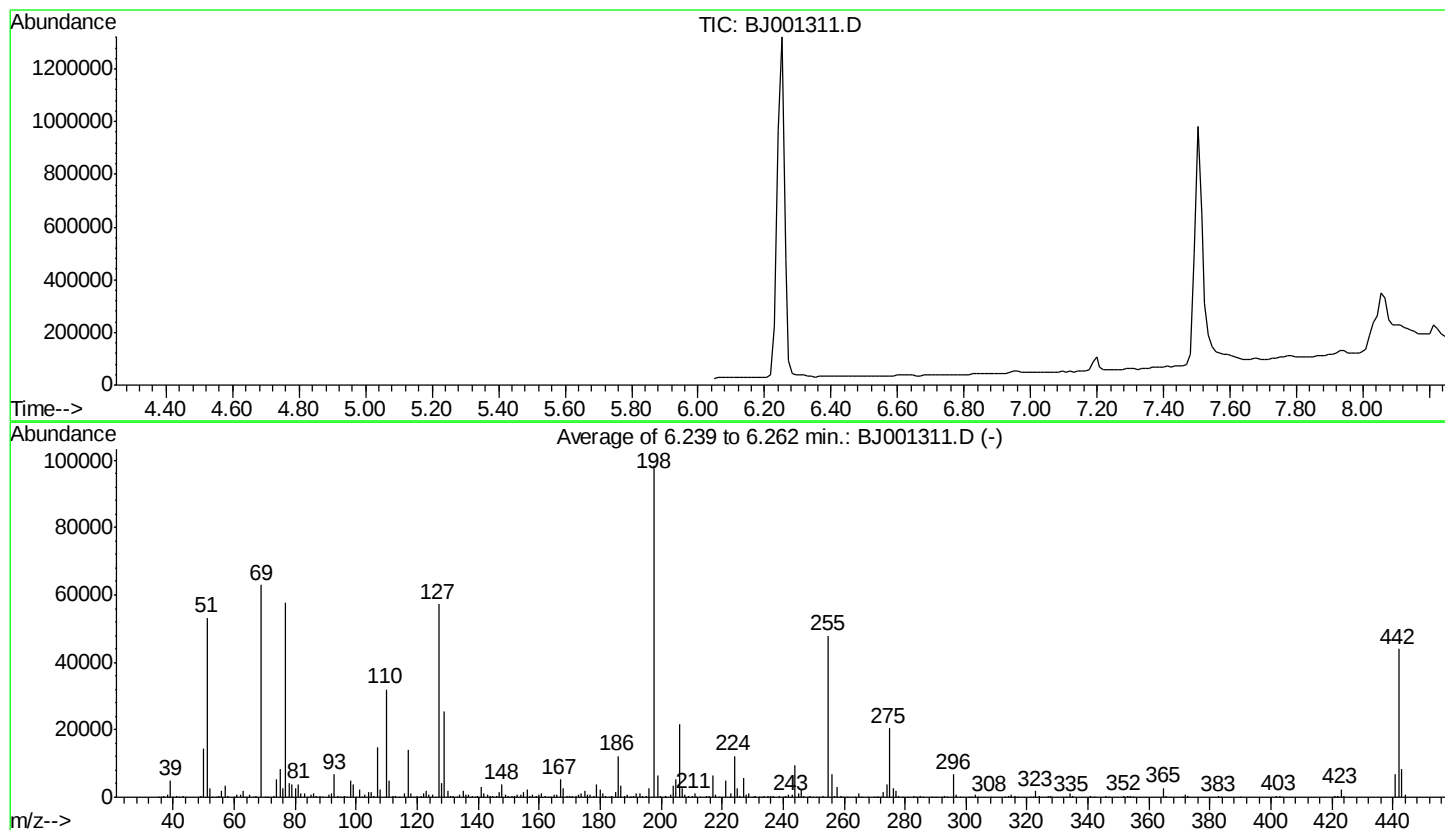

AutoFind: Scans 18, 19, 20; Background Corrected with Scan 13

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	54.2	53304	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	64.0	62896	PASS
70	69	0.00	2	0.3	196	PASS
127	198	40	60	58.3	57319	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	98336	PASS
199	198	5	9	6.5	6402	PASS
275	198	10	30	20.8	20492	PASS
365	198	1	100	2.9	2840	PASS
441	443	0.01	100	82.3	6784	PASS
442	198	40	100	44.7	44002	PASS
443	442	17	23	18.7	8245	PASS