Quantitation Report (Not Reviewed)

Data File : H:\VOL1\GCMSDATA\J\121210\BJ001333.D Vial: 7
Acq On : 10 Dec 2012 20:20 Operator: HLM
Sample : D5081-03 Inst : BNA J
Misc : WATER BNA J HLM Multiplr: 1.00
MS Integration Params: rteint.p
Quant Time: Dec 12 13:00 2012 Quant Results File: BJ121012.RES

**Instrument :** BNA_J
**ClientSampleId :** NMB08A-120512F

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ121012.M (RTE Integrator)
Title : CWA degredation products by GCMS
Last Update : Mon Dec 10 18:28:25 2012
Response via : Initial Calibration
DataAcq Meth : CWAJ

| Internal Standards | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|---|---|---|---|---|---|---|
| 1) 1,4-Dichlorobenzene-d4 | 4.37 | 152 | 136872 | 2.00 | ug/mL | 0.00 |
| 6) Naphthalene-d8 | 5.64 | 136 | 641704 | 2.00 | ug/mL | 0.00 |
| **System Monitoring Compounds** | | | | | | |
| 10) Tripropylphosphate | 6.71 | 99 | 142962 | 0.54 | ug/mL | 0.00 |
| Spiked Amount 0.500 | Range 70 - 130 | | Recovery = 108.00% | | | |
| 12) 2-Bromothioanisole | 6.92 | 204 | 259181 | 4.05 | ug/mL | 0.00 |
| Spiked Amount 5.000 | Range 70 - 130 | | Recovery = 81.00% | | | |
| **Target Compounds** | | | | | | Qvalue |
| 14) p-Chlorophenylmethylsulfon | 7.76 | 111 | 1728 | 0.01 | ug/mL# | 38 |

(#) = qualifier out of range (m) = manual integration

Quantitation Report

Data File : H:\VOL1\GCMSDATA\J\121210\BJ001333.D Vial: 7
Acq On : 10 Dec 2012 20:20 Operator: HLM
Sample : D5081-03 Inst : BNA J
Misc : WATER BNA J HLM Multiplr: 1.00
MS Integration Params: rteint.p
Quant Time: Dec 12 13:00 2012 Quant Results File: BJ121012.RES

**Instrument :**
BNA_J
**ClientSampleId :**
NMB08A-120512F

Method : H:\VOL1\GCMSDATA\J\METHODS\BJ121012.M (RTE Integrator)
Title : CWA degredation products by GCMS
Last Update : Mon Dec 10 18:28:25 2012
Response via : Initial Calibration

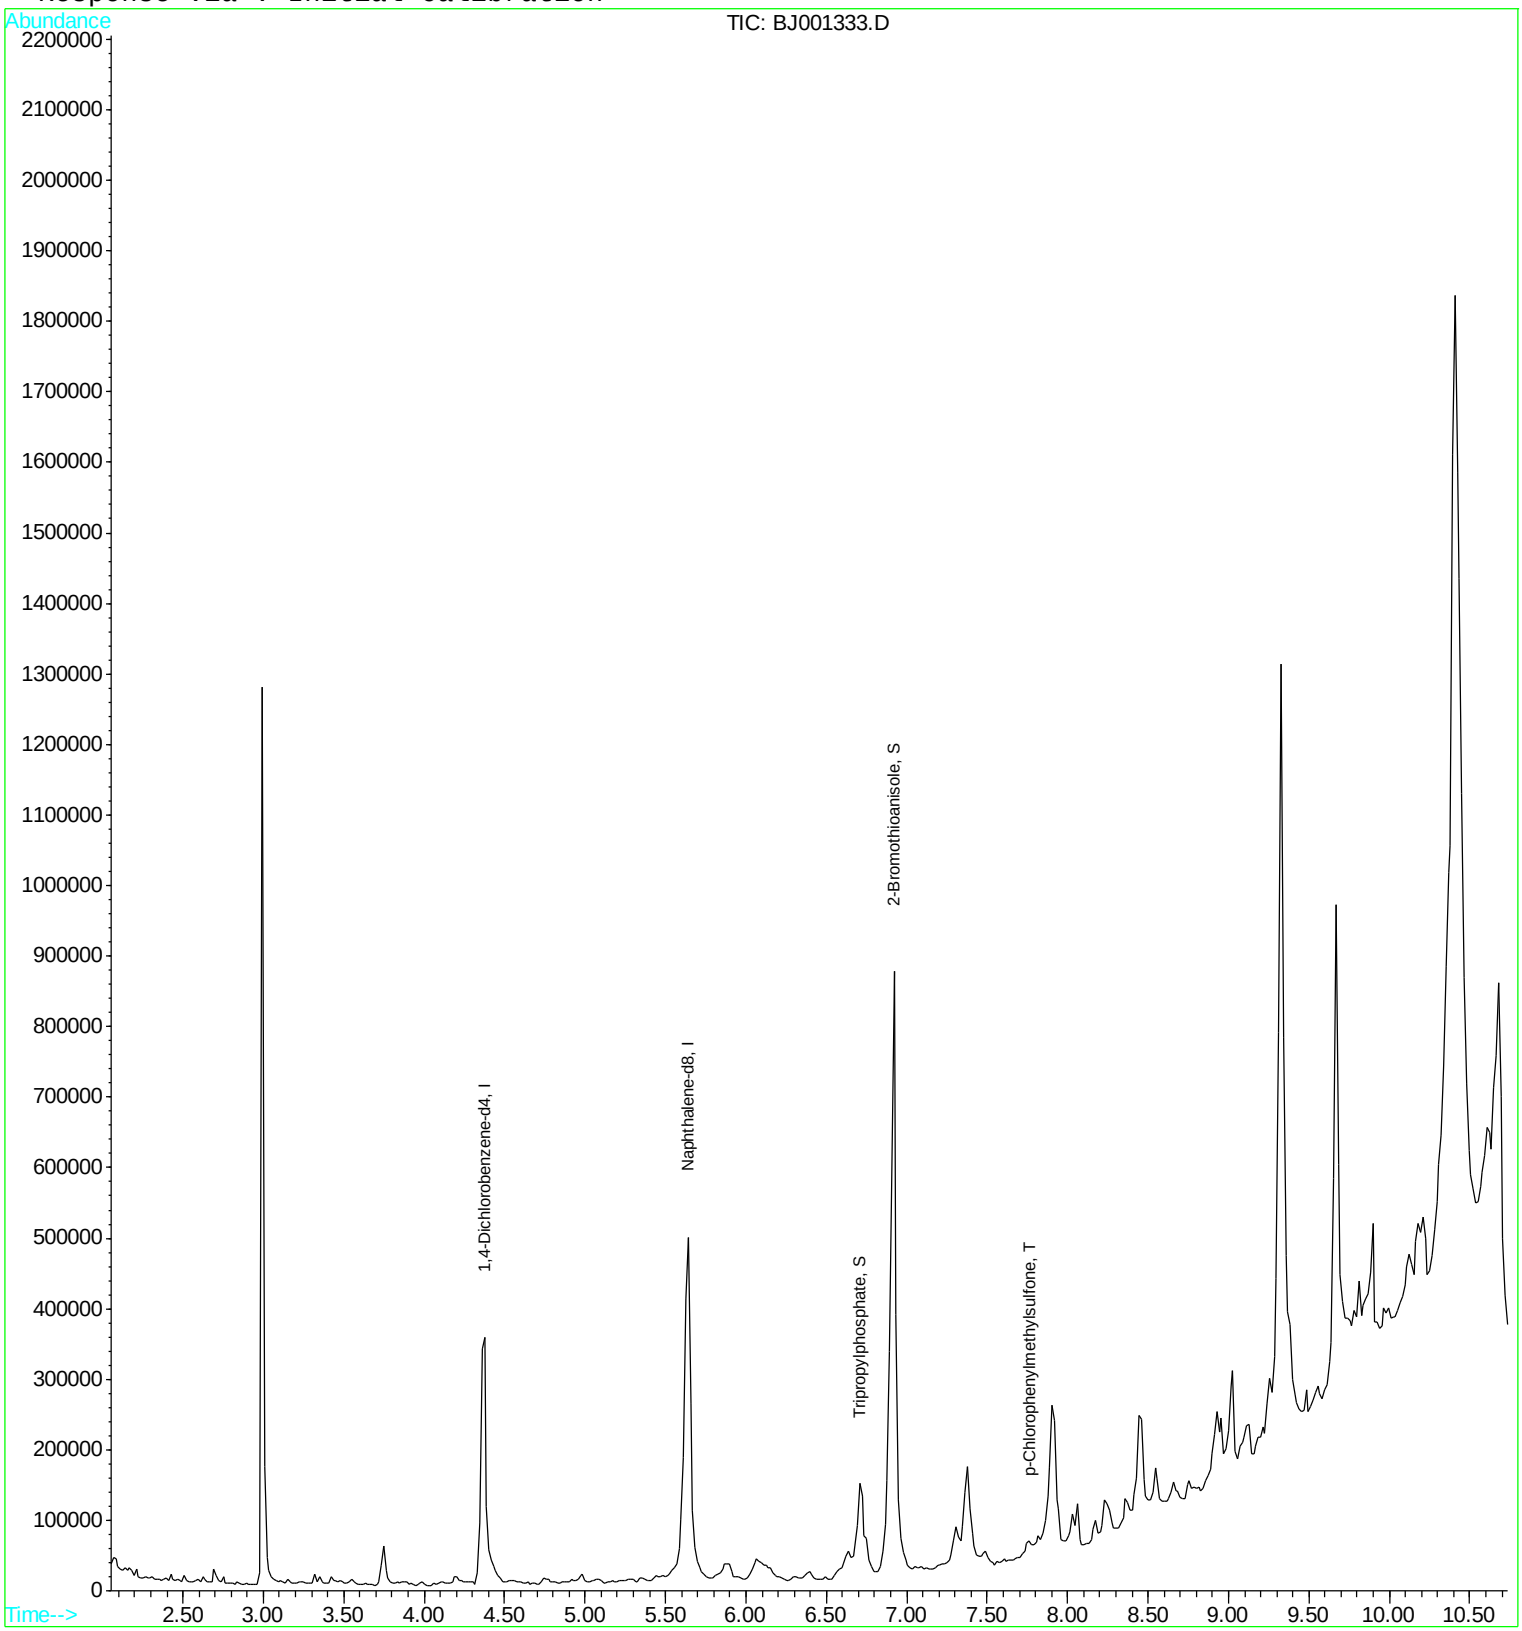

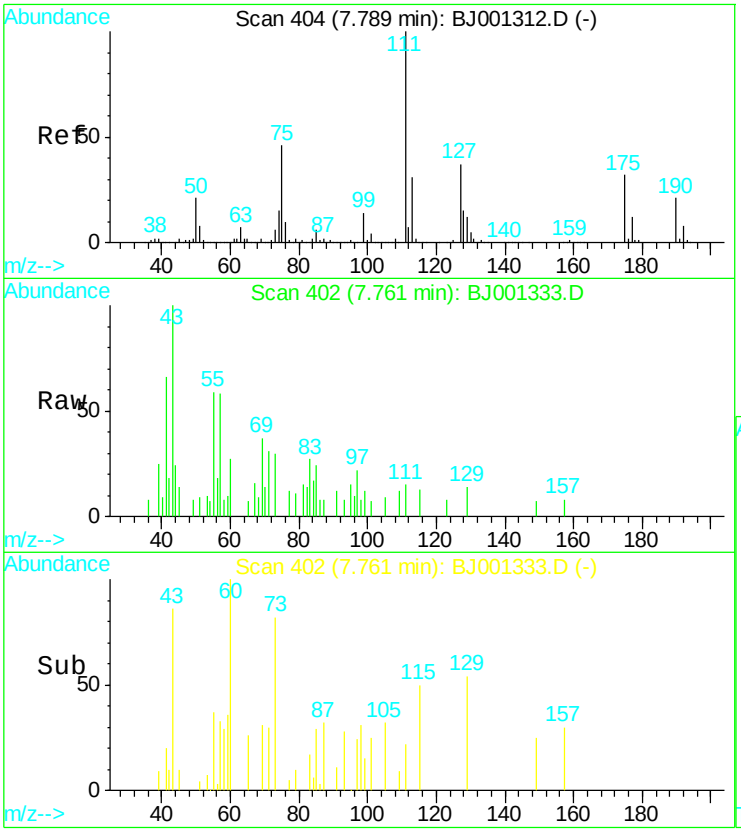


#14
p-Chlorophenylmethylsulfone
Concen: 0.01 ug/mL
RT: 7.76 min  Scan# 402
Delta R.T.  -0.02 min
Lab File:  BJ001333.D
Acq: 10 Dec 2012  20:20

**Instrument :**
BNA_J
**ClientSampleId :**
NMB08A-120512F

Tgt Ion:111 Resp:  1728

| Ion | Ratio | Lower | Upper |
|---|---|---|---|
| 111 | 100 | | |
| 75 | 0.0 | 27.3 | 67.3# |
| 127 | 0.0 | 17.0 | 57.0# |
| 190 | 0.0 | 0.8 | 40.8# |