


Data Path : Z:\HPCHEM1\BNA_J\data\BJ121012\
 Data File : BJ001320.D
 Acq On : 10 Dec 2012 12:11
 Operator : HLM
 Sample : DFTPP050
 Misc : DFTPP050 BNA_J HLM
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_J
 ClientSampleId :
 DFTPP050

Integration File: rteint.p

Method : S:\HPCHEM1\BNA_J\method\BJ121012.M
 Title : CWA degradation products by GCMS
 Last Update : Mon Dec 10 18:30:47 2012

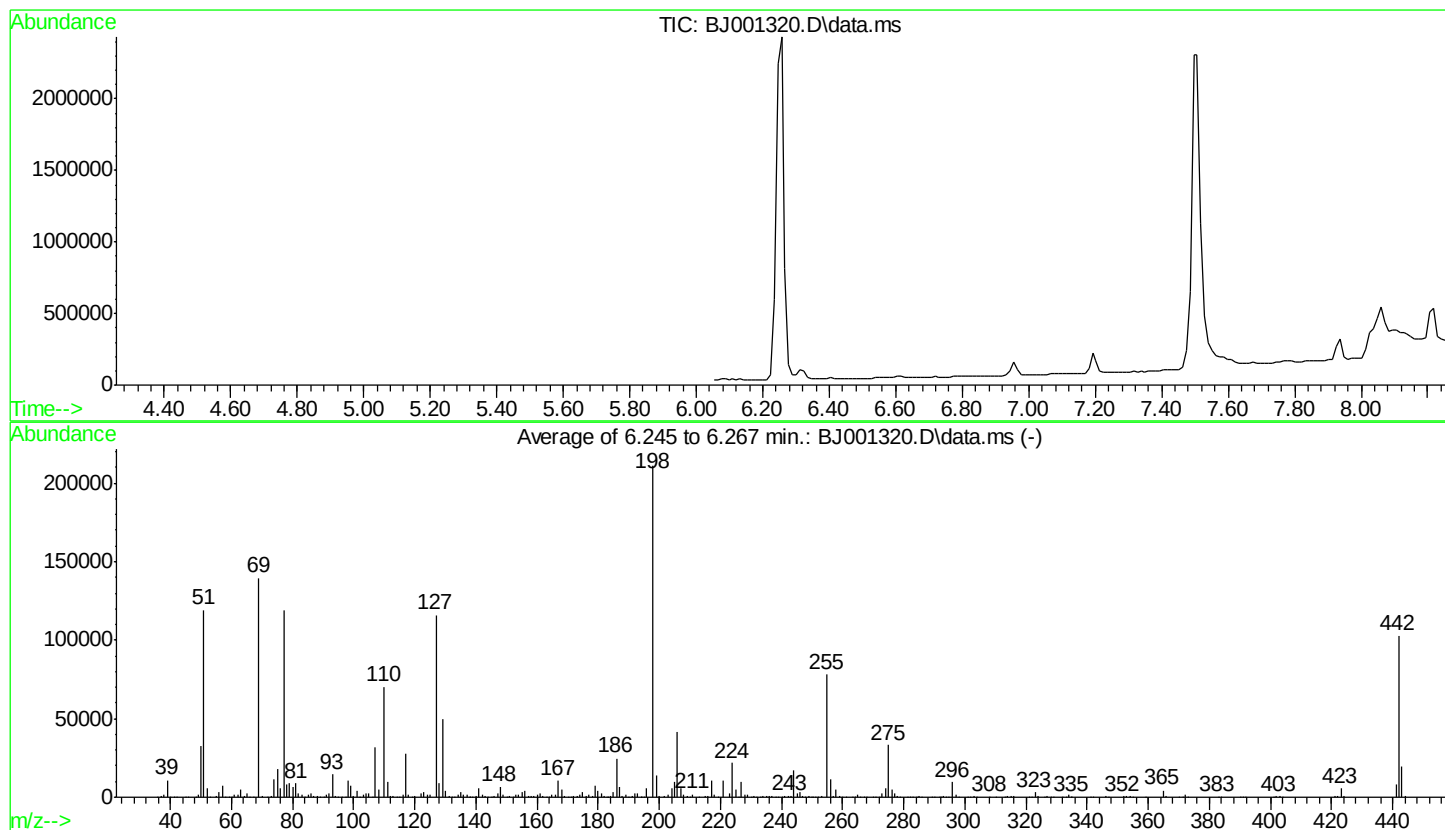

AutoFind: Scans 18, 19, 20; Background Corrected with Scan 13

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	56.6	119423	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	66.2	139730	PASS
70	69	0.00	2	0.4	495	PASS
127	198	40	60	55.0	116082	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	211168	PASS
199	198	5	9	6.7	14180	PASS
275	198	10	30	15.8	33266	PASS
365	198	1	100	2.0	4153	PASS
441	443	0.01	100	39.4	7860	PASS
442	198	40	100	48.7	102914	PASS
443	442	17	23	19.4	19943	PASS