

Data File : H:\VOL1\GCMSDATA\J\120608\BJ000942.D

Vial: 8

Acq On : 8 Jun 2012 18:01

Operator: HLM

Sample : PB63665BL

Inst : BNA J

Misc : WATER BNA J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jun 11 15:28 2012

Quant Results File: BJ060812.RES

Quant Method : H:\VOL1\GCMSDATA\J\METHODS\BJ060812.M (RTE Integrator)

Title : CWA degradation products by GCMS

Last Update : Fri Jun 08 15:52:40 2012

Response via : Initial Calibration

DataAcq Meth : CWAJ

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	4.71	152	272389	2.00	ug/mL	0.00
6) Naphthalene-d8	6.00	136	1120191	2.00	ug/mL	0.00
System Monitoring Compounds						
10) Tripropylphosphate	7.00	99	14069	0.03	ug/mL	-0.05
Spiked Amount 0.500	Range	70 - 130	Recovery	=	6.00%#	
12) 2-Bromothioanisole	7.31	204	250257	3.27	ug/mL	0.00
Spiked Amount 5.000	Range	70 - 130	Recovery	=	65.40%#	
Target Compounds						Ovalue
11) p-Chlorophenylmethylsulfid	6.56	158	7288	0.04	ug/mL#	35
13) p-Chlorophenylmethylsulfox	7.98	159	1026	0.05	ug/mL#	1

Data File : H:\VOL1\GCMSDATA\J\120608\BJ000942.D

Vial: 8

Acq On : 8 Jun 2012 18:01

Operator: HLM

Sample : PB63665BL

Inst : BNA J

Misc : WATER BNA J HLM

Multiplr: 1.00

MS Integration Params: rteint.p

Quant Time: Jun 11 15:28 2012


Quant Results File: BJ060812.RES




Method : H:\VOL1\GCMSDATA\J\METHODS\BJ060812.M (RTE Integrator)

Title : CWA degradation products by GCMS

Last Update : Fri Jun 08 15:52:40 2012





Response via : Initial Calibration

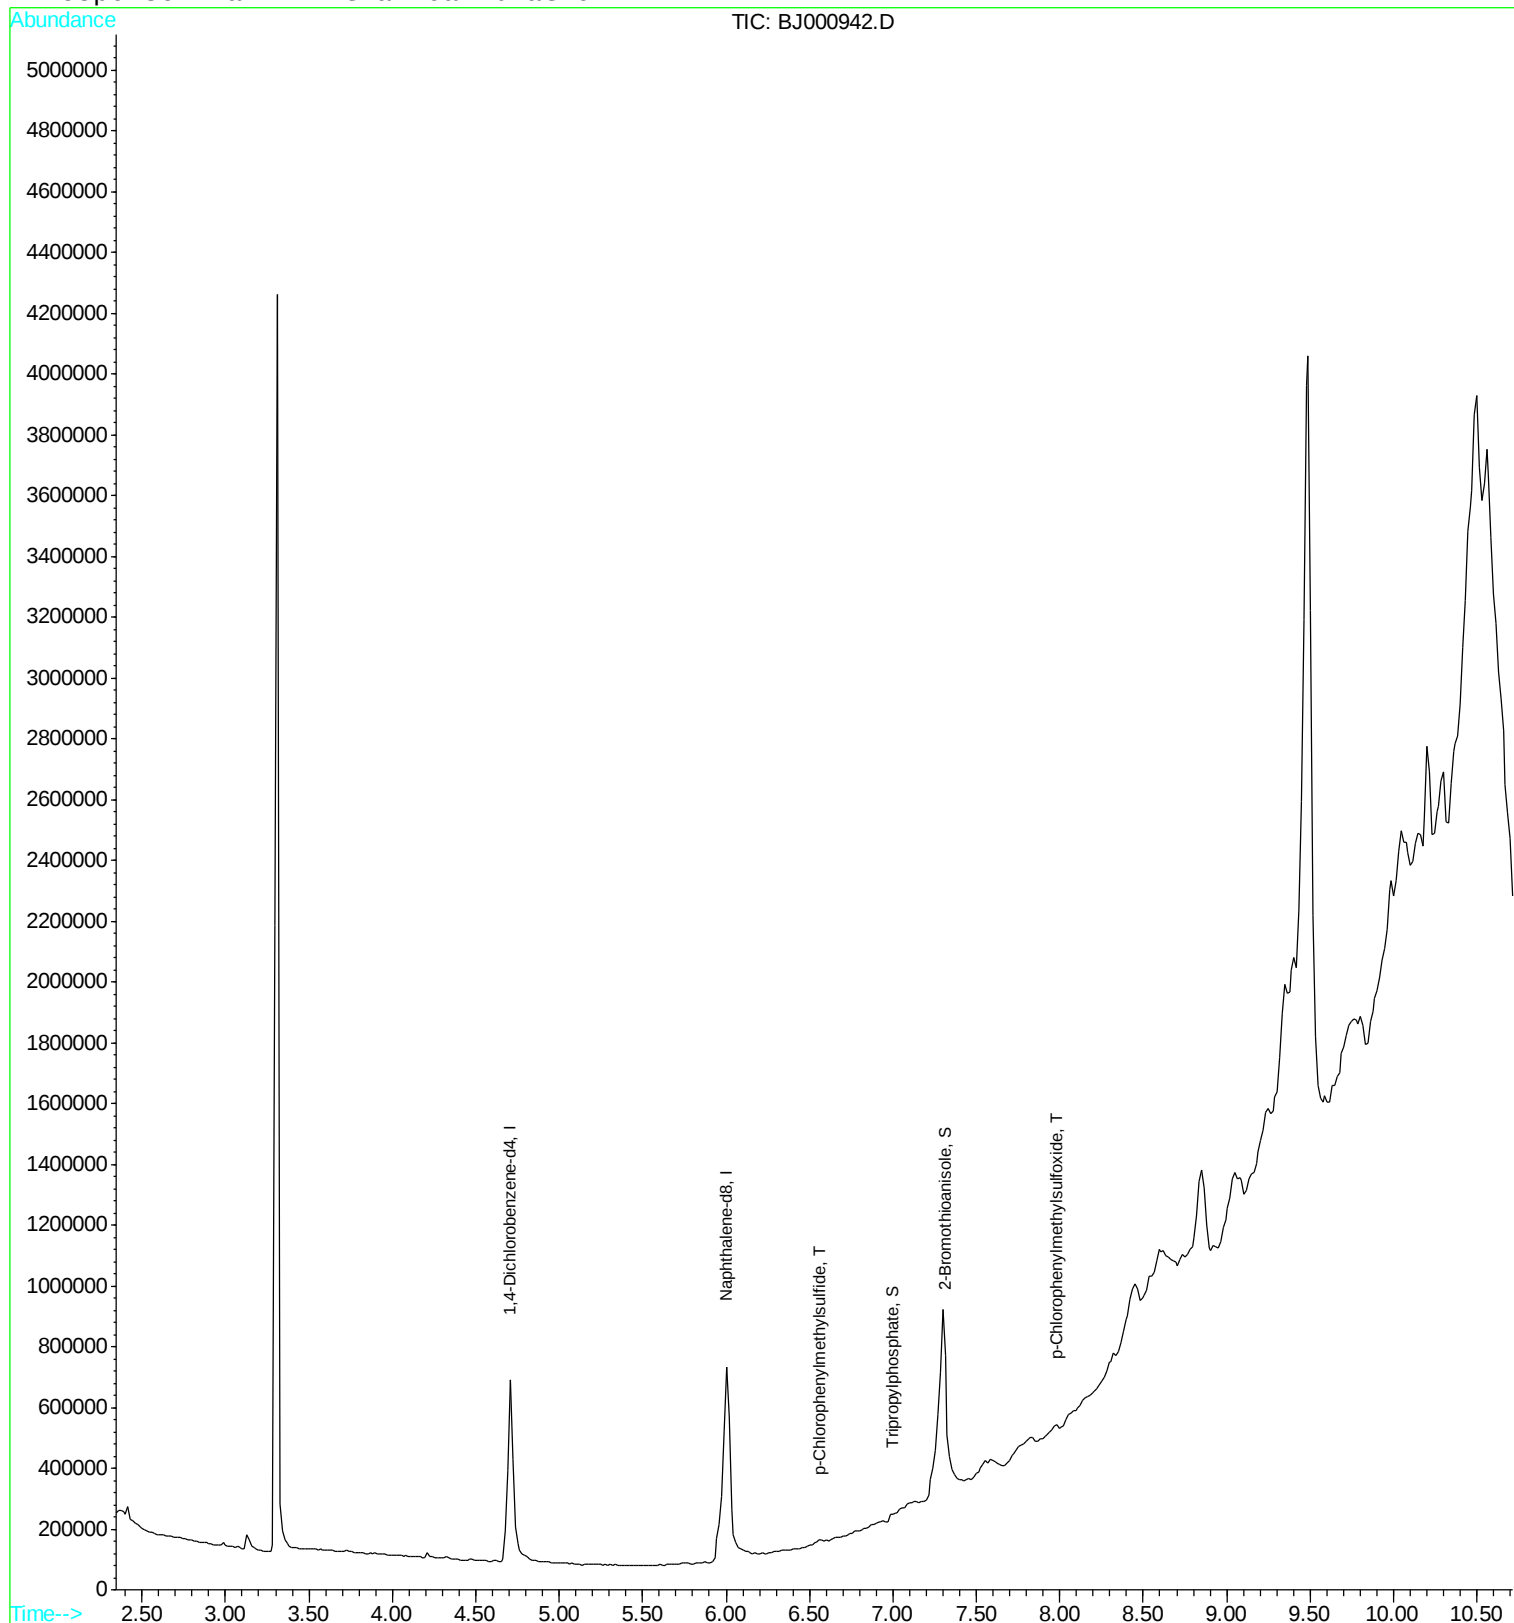

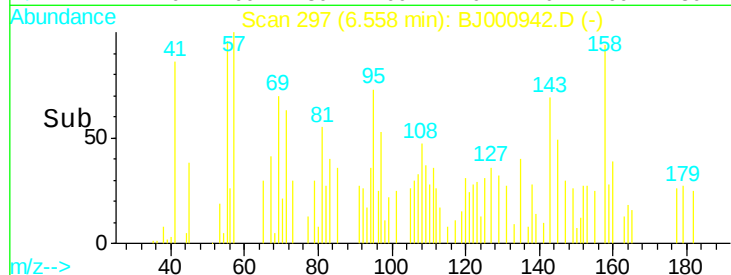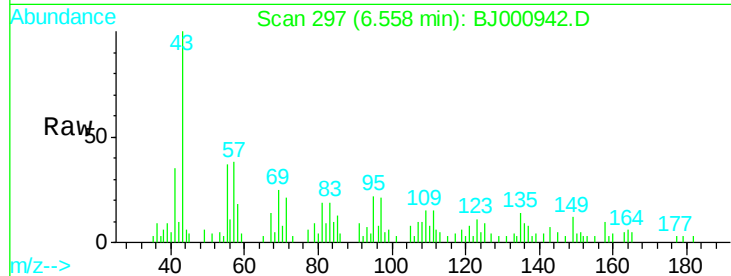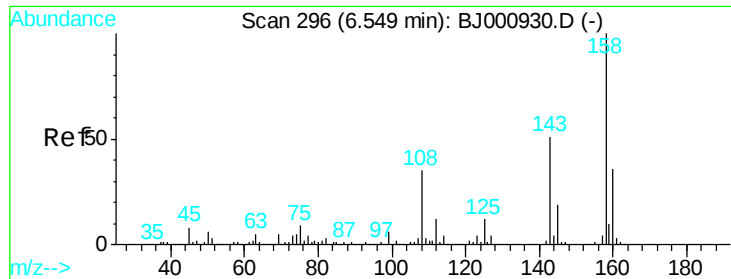

#11
p-Chlorophenylmethylsulfide
Concen: 0.04 ug/mL
RT: 6.56 min Scan# 297
Delta R.T. 0.01 min
Lab File: BJ000942.D
Acq: 8 Jun 2012 18:01

Tgt Ion:158 Resp: 7288
Ion Ratio Lower Upper
158 100
143 73.7 31.3 71.3#
108 97.1 14.9 54.9#
45 40.6 0.0 28.5#

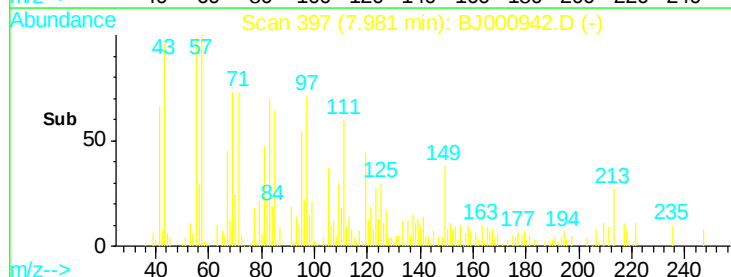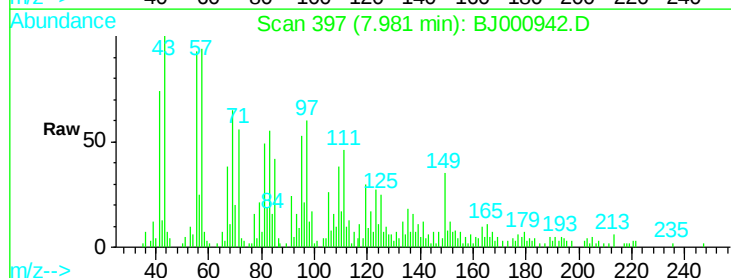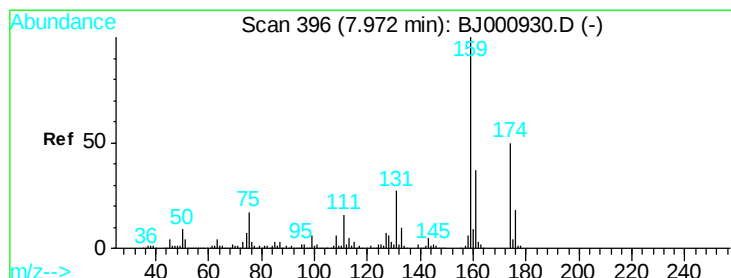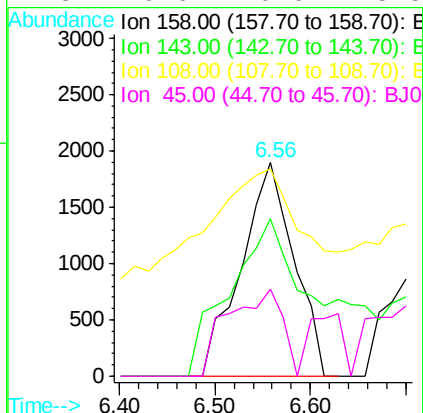

#13
p-Chlorophenylmethylsulfoxide
Concen: 0.05 ug/mL
RT: 7.98 min Scan# 397
Delta R.T. 0.01 min
Lab File: BJ000942.D
Acq: 8 Jun 2012 18:01

Tgt Ion:159 Resp: 1026
Ion Ratio Lower Upper
159 100
174 0.0 27.0 67.0#
108 67.5 0.0 28.3#
50 86.1 0.0 36.8#

